


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF040419\
 Data File : VF062157.D
 Acq On : 4 Apr 2019 12:32
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F040419S.M
 Title : SW846 8260
 Last Update : Fri Apr 05 05:27:08 2019

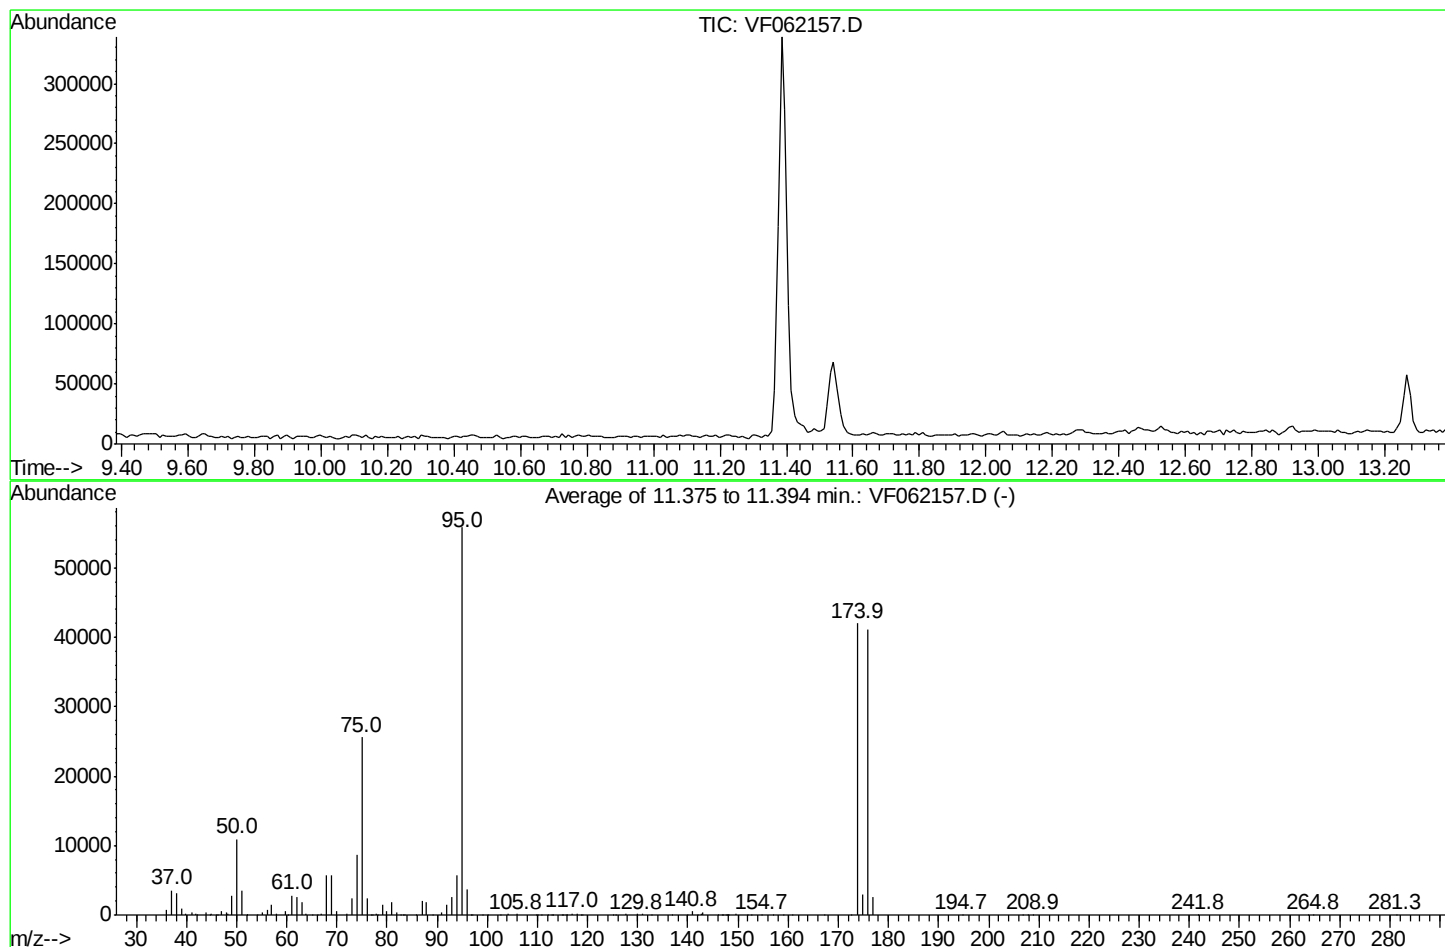

AutoFind: Scans 1101, 1102, 1103; Background Corrected with Scan 1096

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	10943	PASS
75	95	30	60	45.9	25613	PASS
95	95	100	100	100.0	55834	PASS
96	95	5	9	6.7	3722	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.2	41994	PASS
175	174	5	9	6.9	2880	PASS
176	174	95	101	97.9	41096	PASS
177	176	5	9	6.4	2646	PASS