




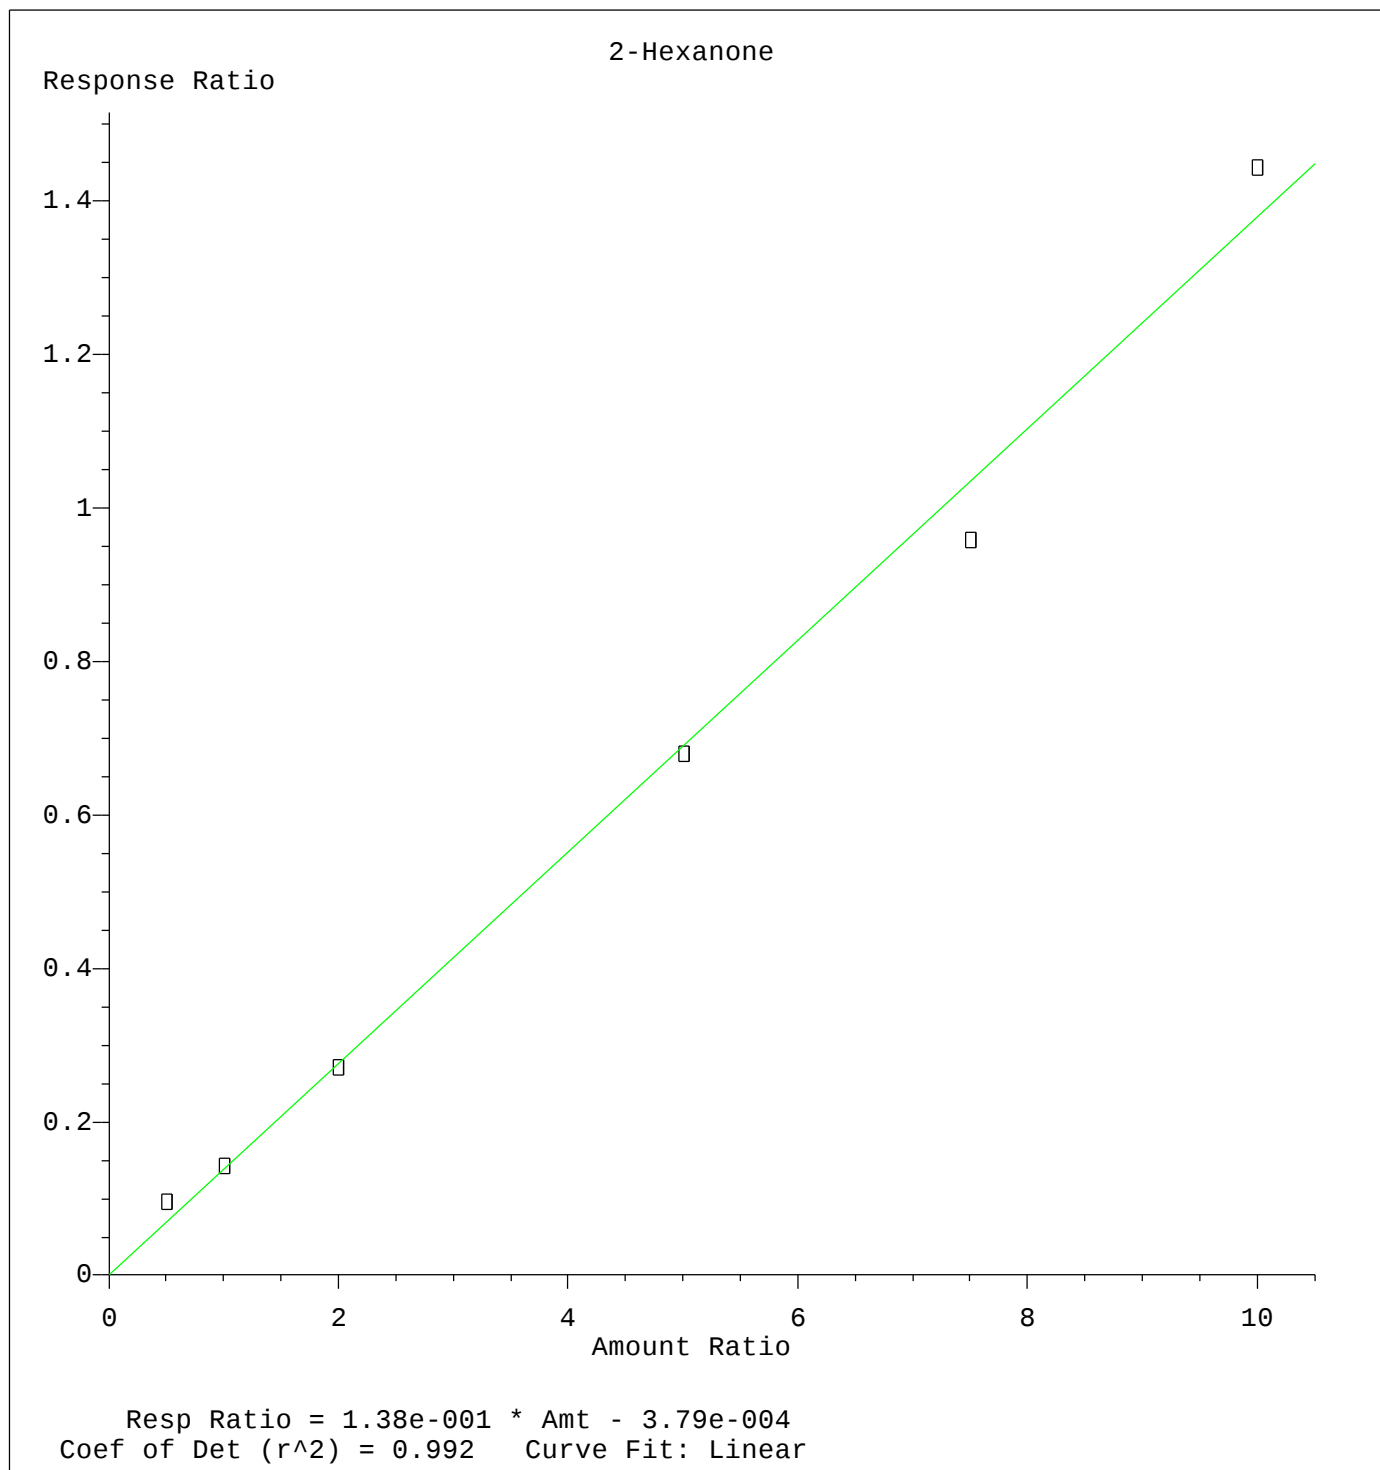


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
Calibration Table Last Updated: Thu Apr 18 07:43:02 2019

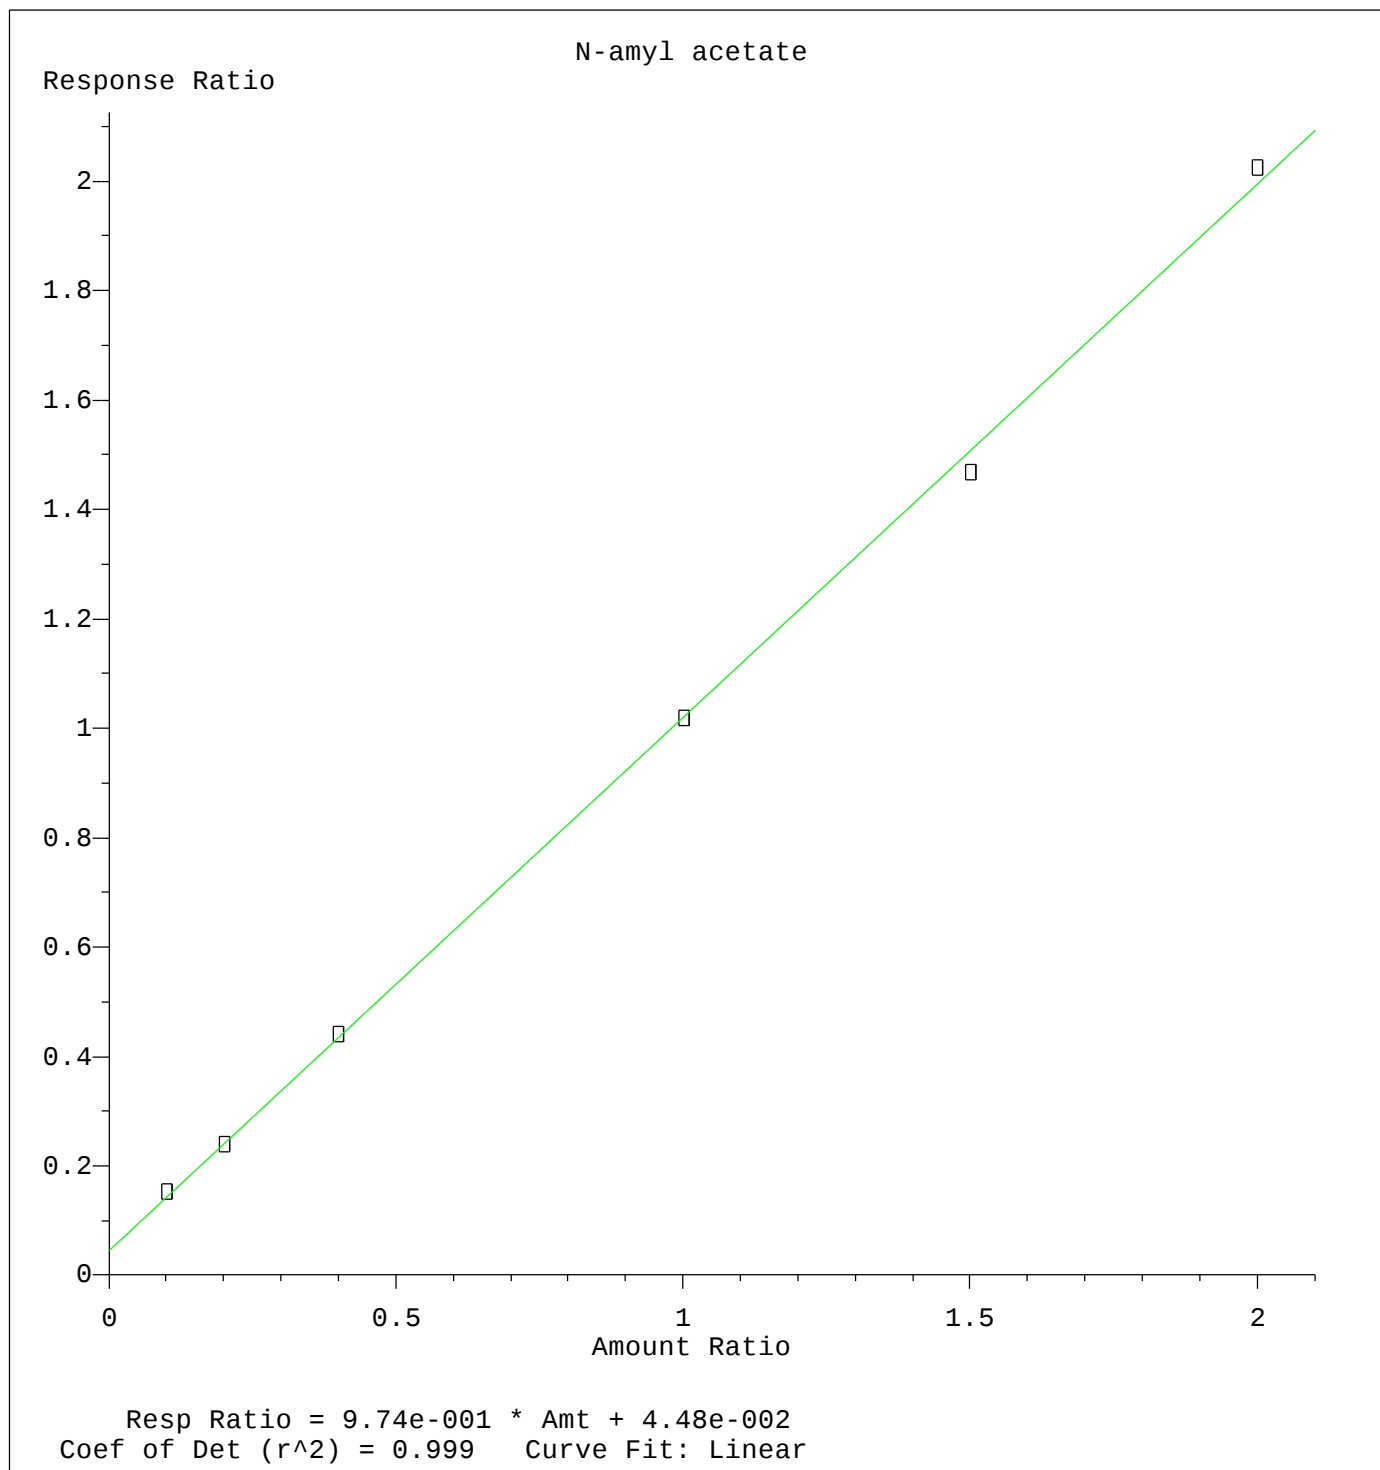


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
Calibration Table Last Updated: Thu Apr 18 07:43:02 2019

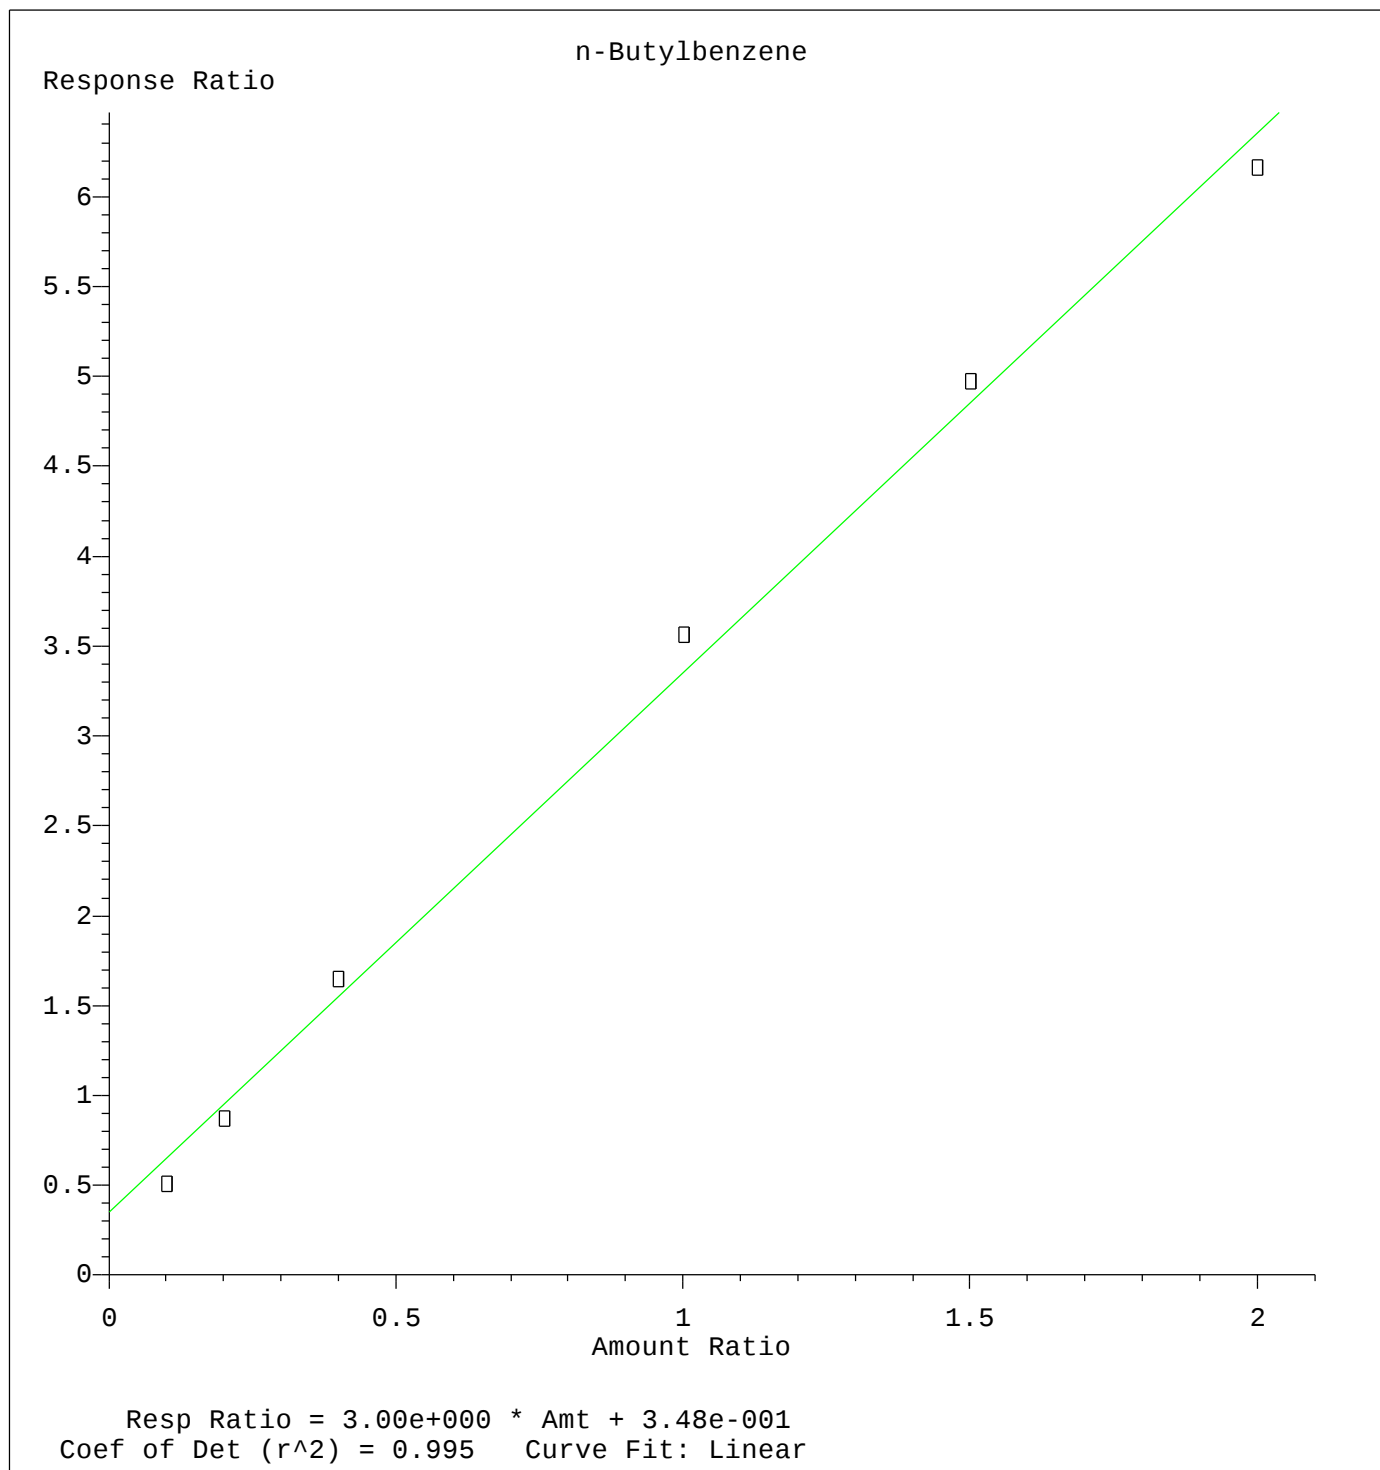

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
Calibration Table Last Updated: Thu Apr 18 07:43:02 2019

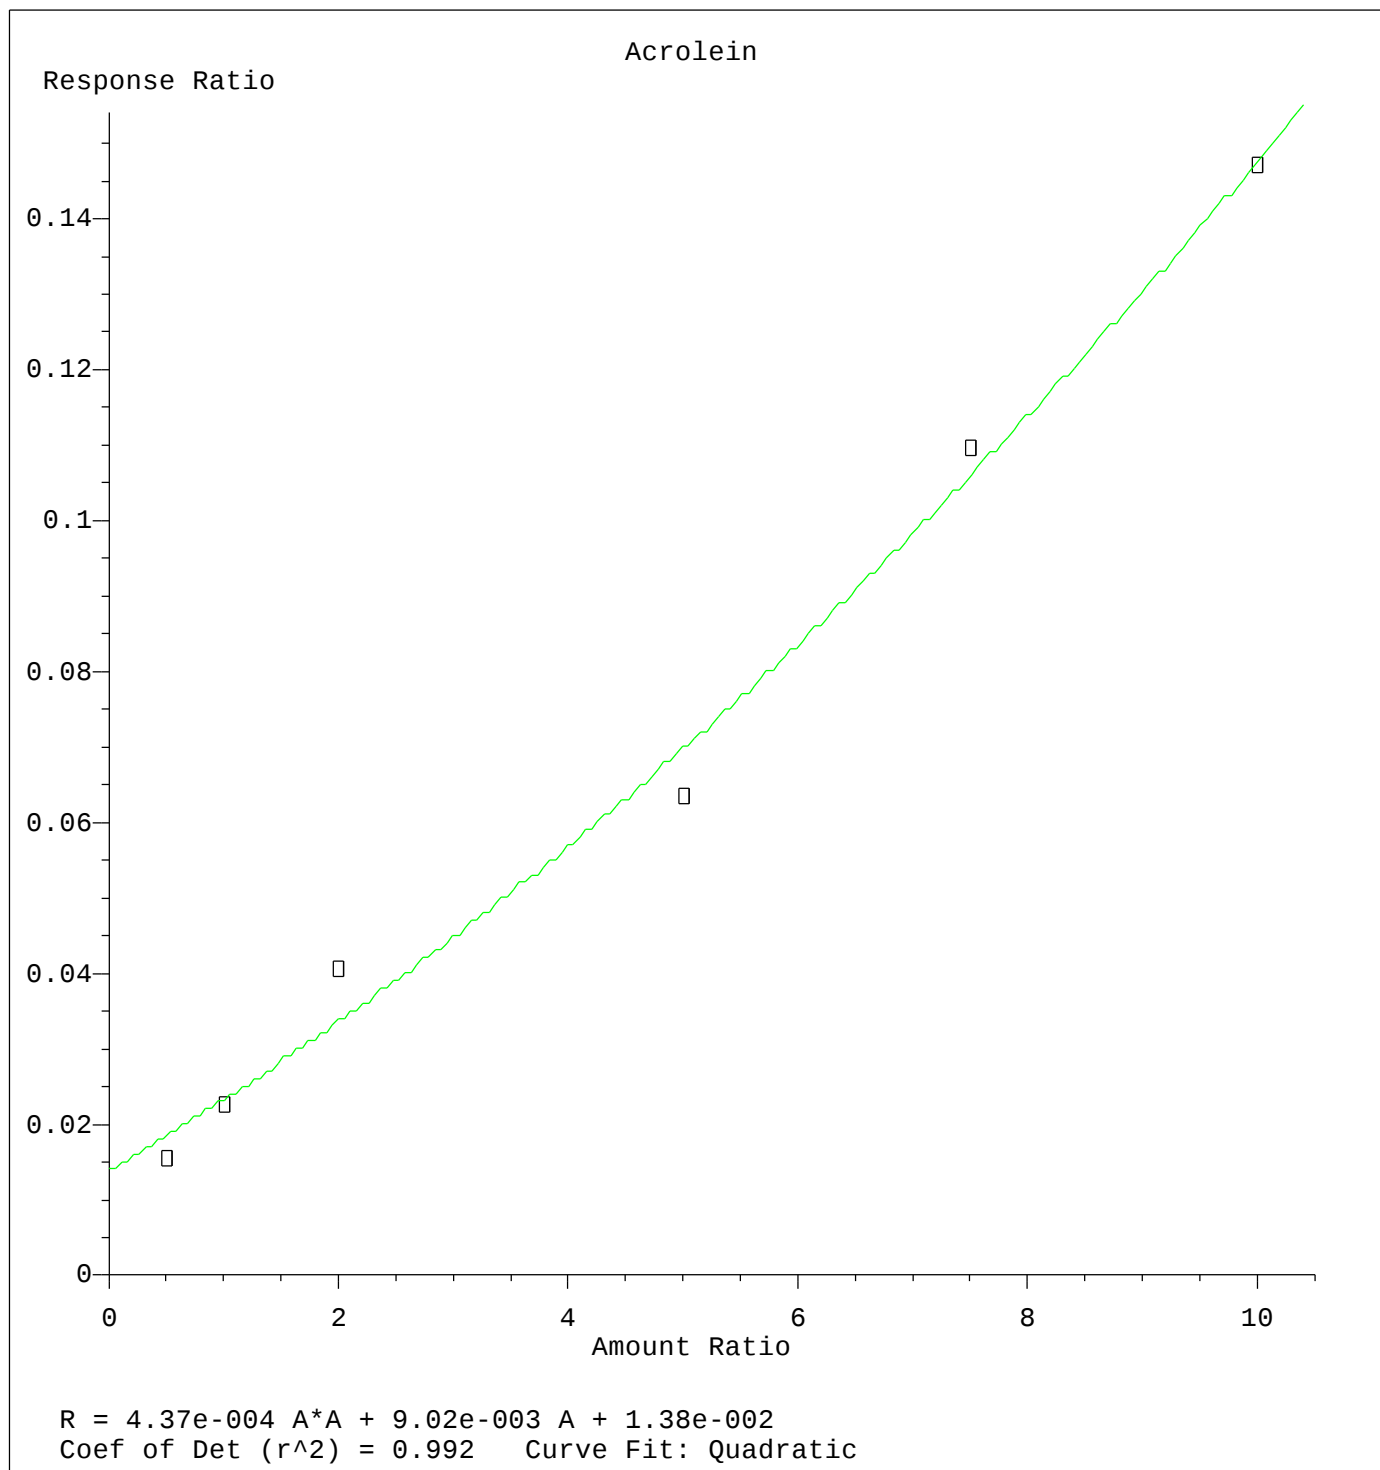


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
Calibration Table Last Updated: Thu Apr 18 07:43:02 2019

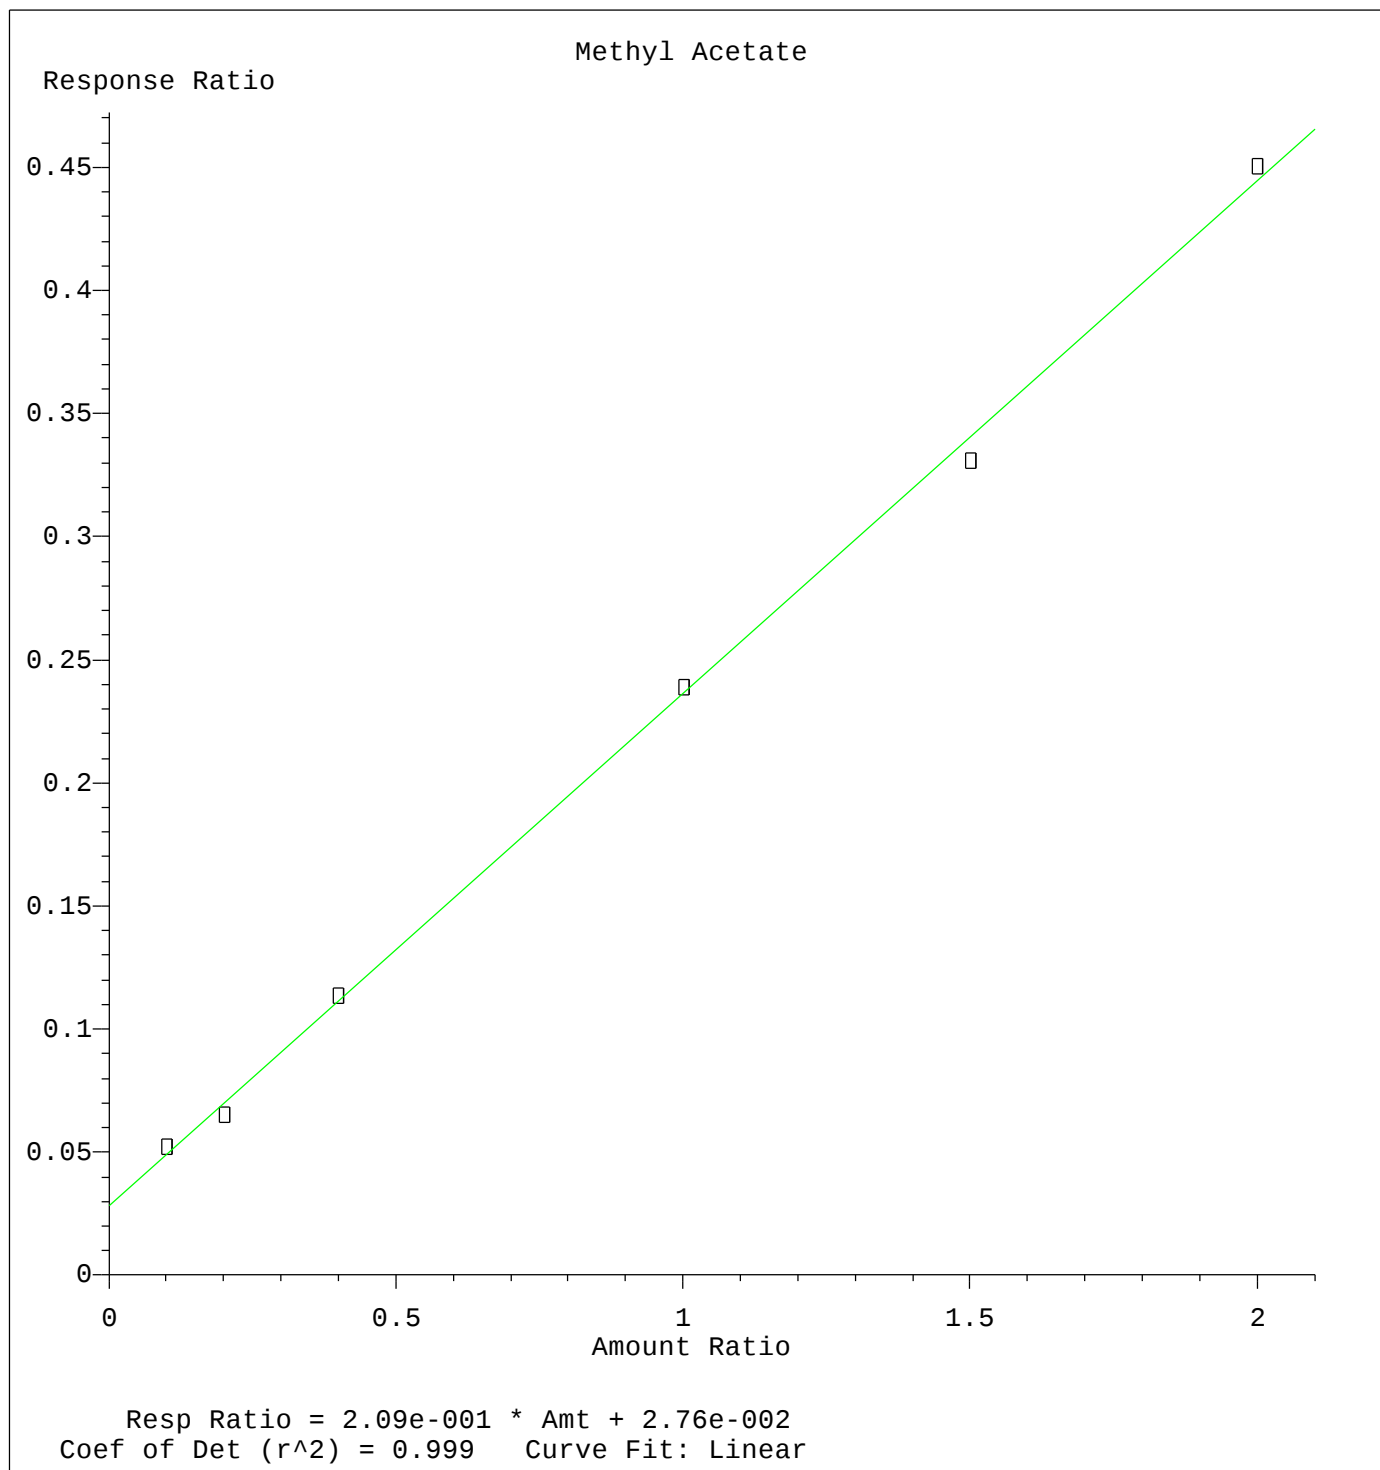

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
Calibration Table Last Updated: Thu Apr 18 07:43:02 2019

Methylene Chloride

Response Ratio

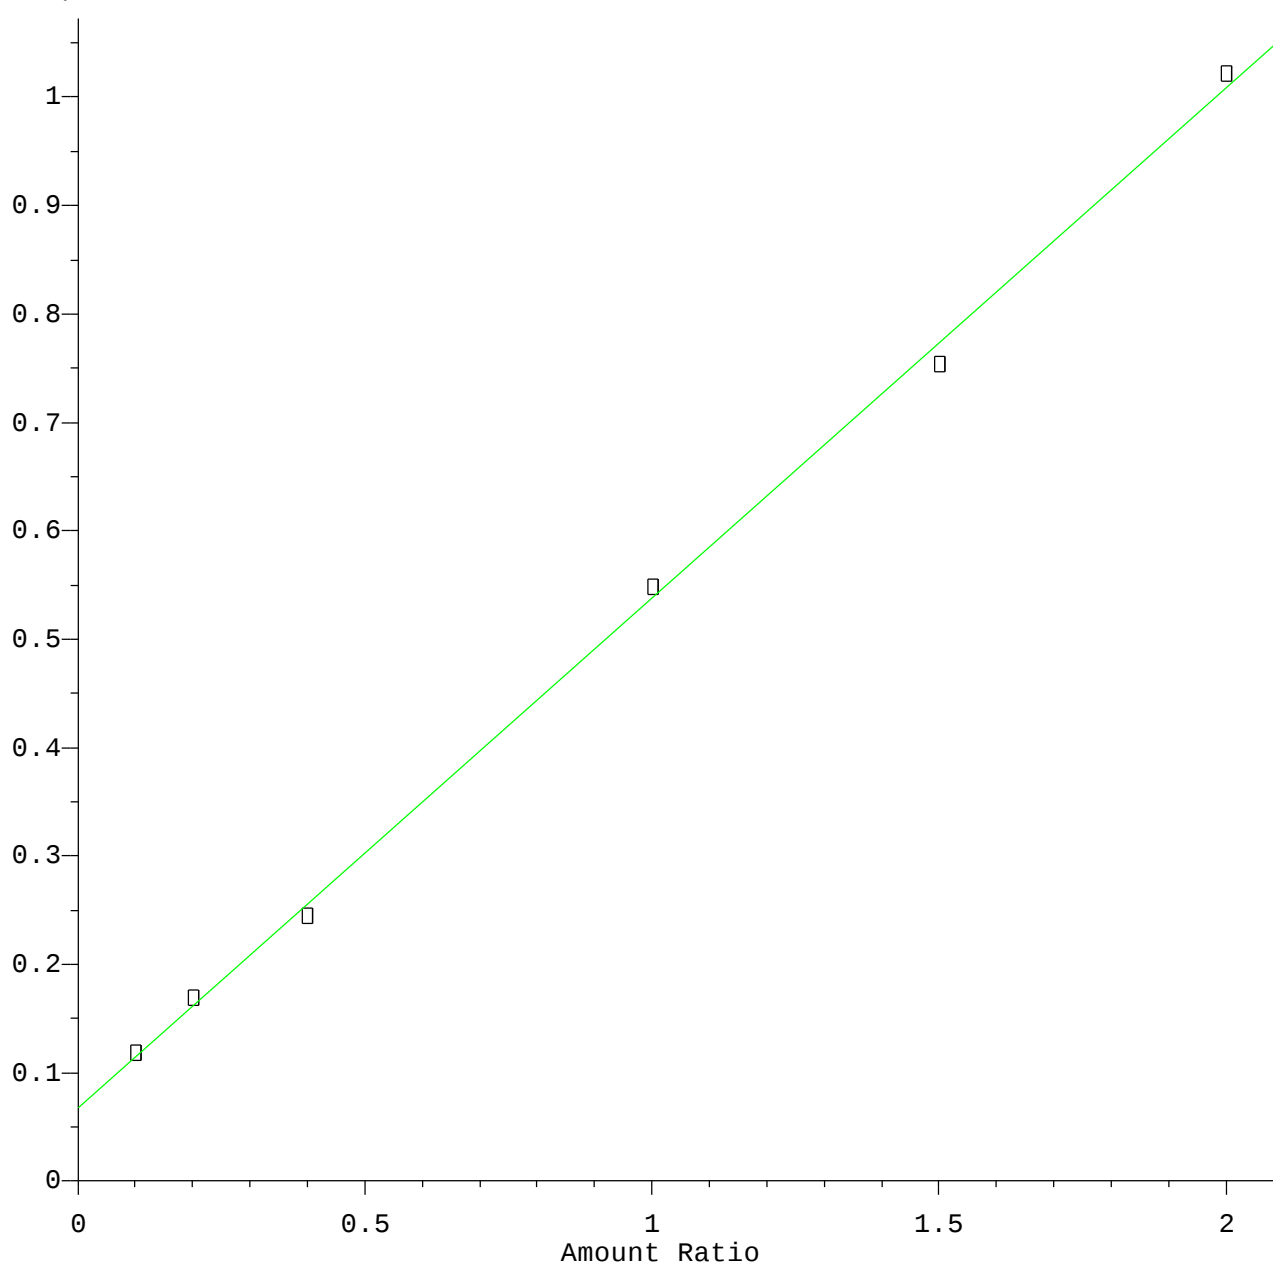

Resp Ratio = $4.71 \times 10^{-1} \times \text{Amt} + 6.74 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
Calibration Table Last Updated: Thu Apr 18 07:43:02 2019