


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF041719\
Data File : VF062189.D
Acq On : 17 Apr 2019 16:01
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
Title : SW846 8260
Last Update : Thu Apr 18 07:43:02 2019

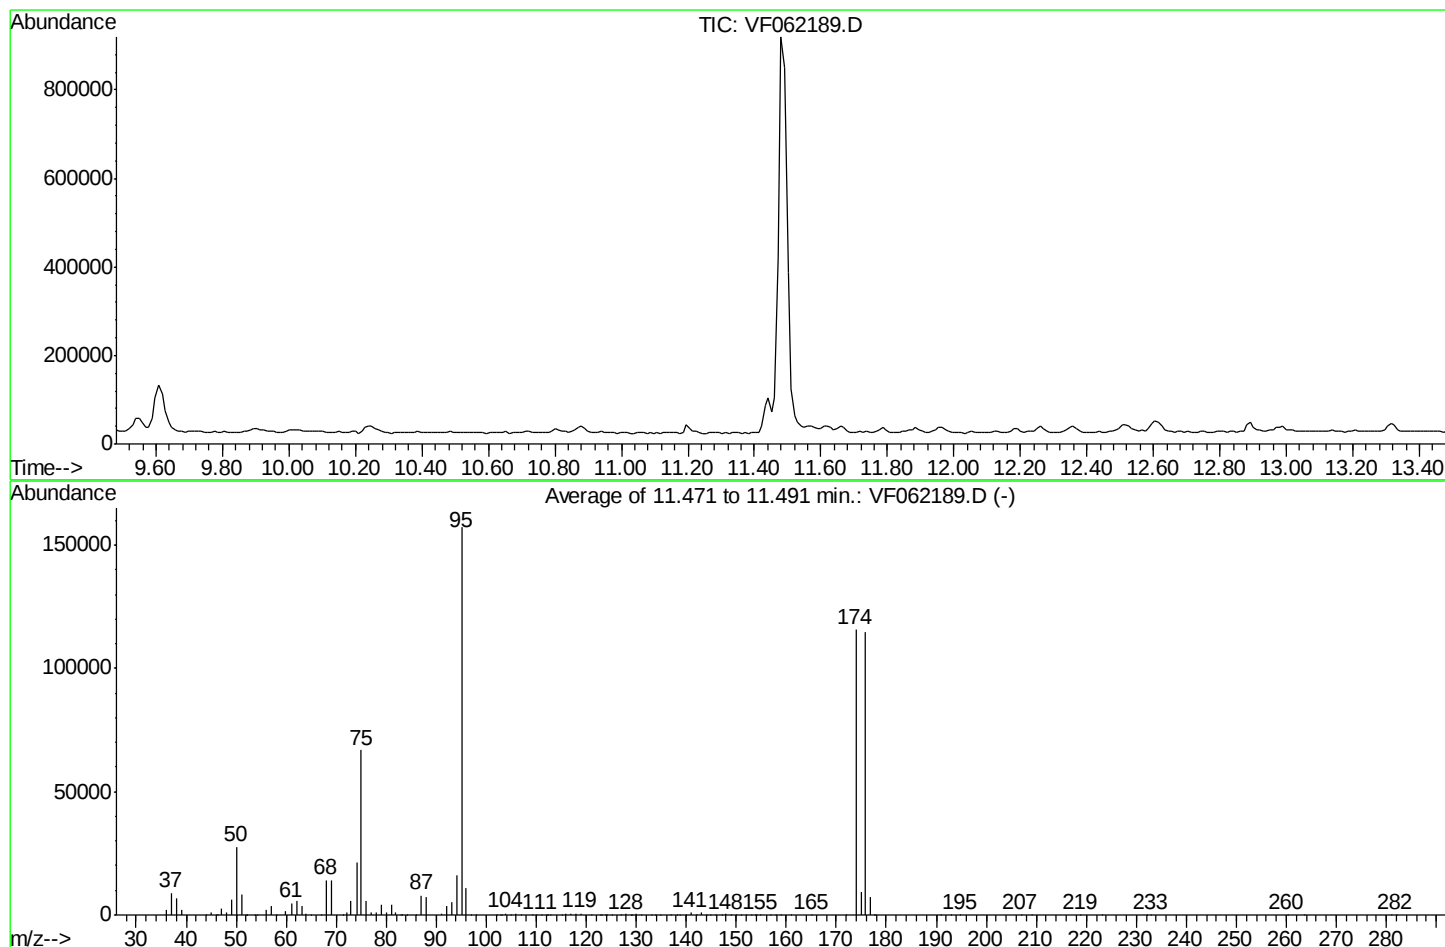

AutoFind: Scans 1110, 1111, 1112; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	27749	PASS
75	95	30	60	42.6	66944	PASS
95	95	100	100	100.0	157180	PASS
96	95	5	9	6.9	10889	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.6	115677	PASS
175	174	5	9	8.1	9324	PASS
176	174	95	101	99.3	114832	PASS
177	176	5	9	6.5	7456	PASS