


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF041819\
 Data File : VF062197.D
 Acq On : 18 Apr 2019 9:46
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
 Title : SW846 8260
 Last Update : Fri Apr 19 03:56:19 2019

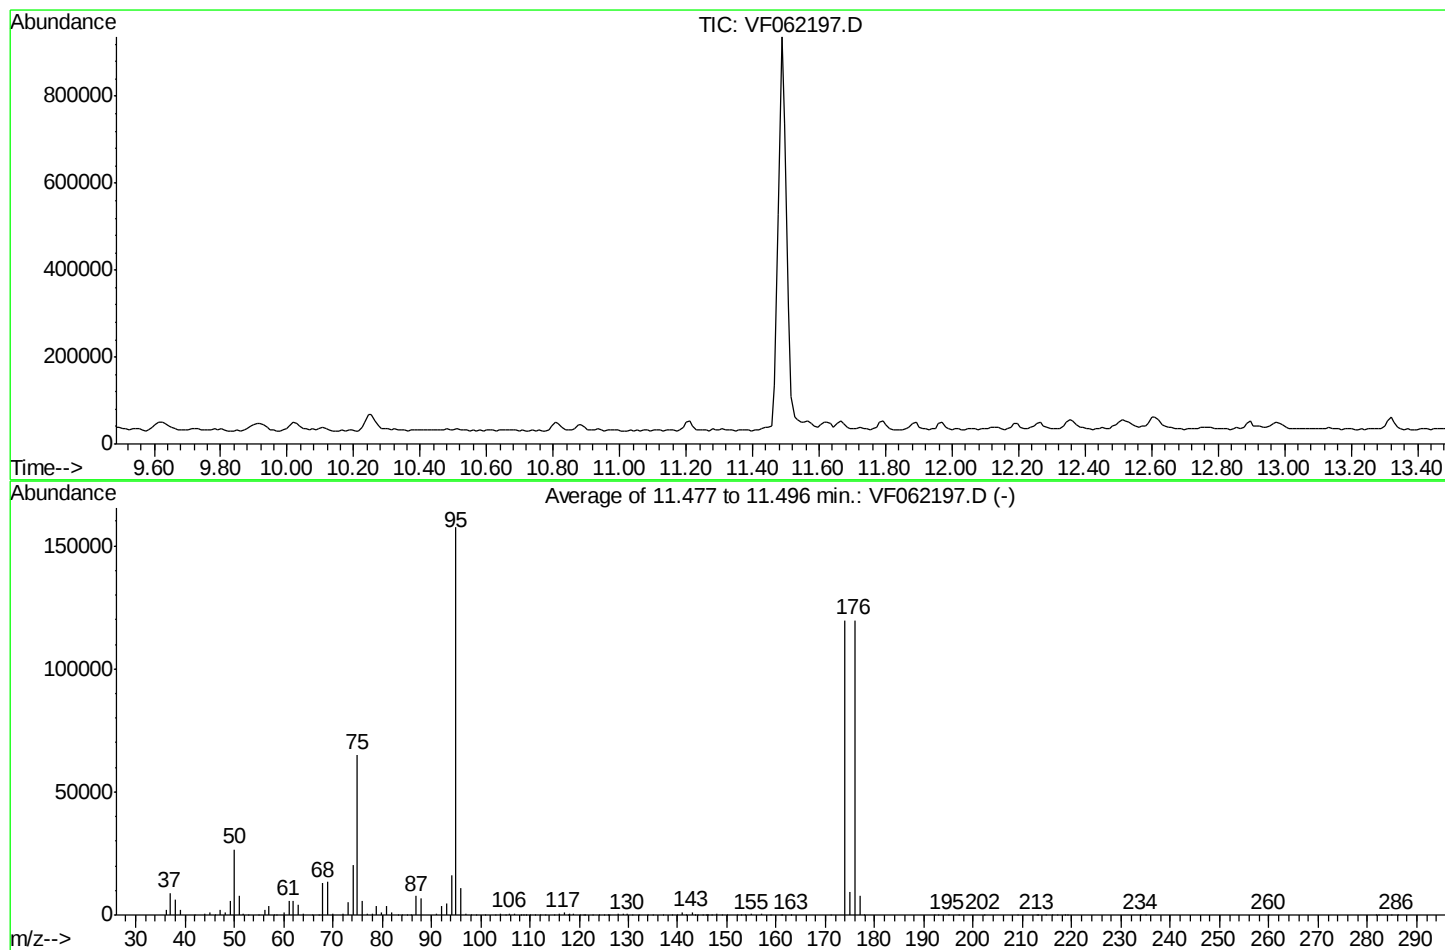

AutoFind: Scans 1110, 1111, 1112; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	26553	PASS
75	95	30	60	41.4	65273	PASS
95	95	100	100	100.0	157557	PASS
96	95	5	9	7.0	11040	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.0	119696	PASS
175	174	5	9	8.0	9552	PASS
176	174	95	101	100.1	119842	PASS
177	176	5	9	6.7	8027	PASS