


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF041919\
Data File : VF062217.D
Acq On : 19 Apr 2019 9:48
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
Title : SW846 8260
Last Update : Fri Apr 19 23:52:01 2019

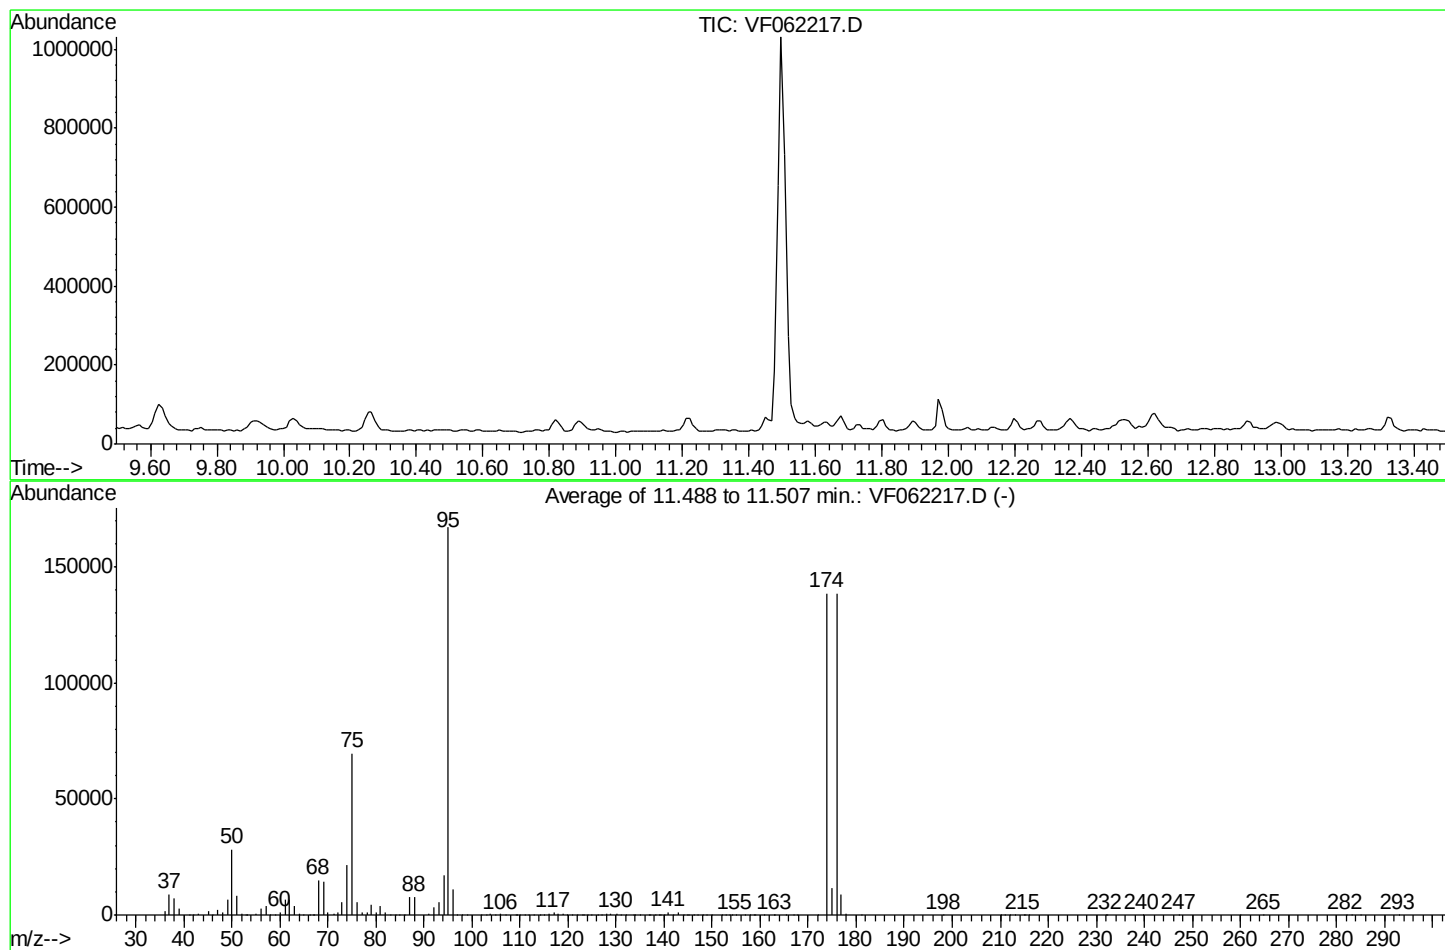

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1101

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	28394	PASS
75	95	30	60	41.7	69626	PASS
95	95	100	100	100.0	166990	PASS
96	95	5	9	6.6	11084	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.0	138605	PASS
175	174	5	9	8.2	11422	PASS
176	174	95	101	99.8	138325	PASS
177	176	5	9	6.6	9090	PASS