


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF042219\
 Data File : VF062237.D
 Acq On : 22 Apr 2019 9:18
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F041719S.M
 Title : SW846 8260
 Last Update : Fri Apr 19 23:52:01 2019

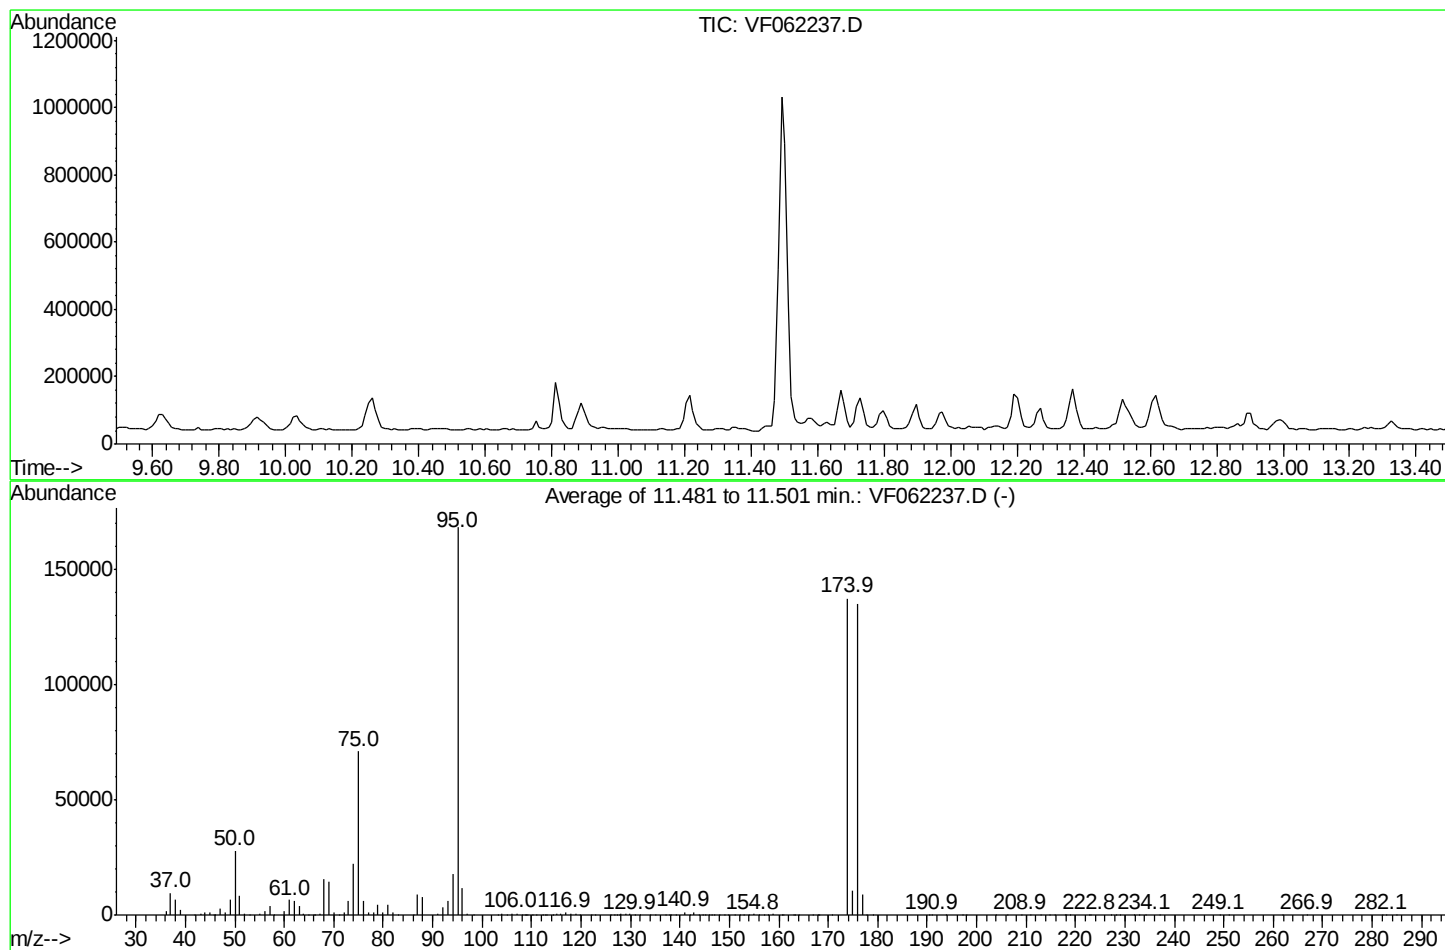

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	27848	PASS
75	95	30	60	42.2	70947	PASS
95	95	100	100	100.0	168296	PASS
96	95	5	9	7.0	11709	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.6	137397	PASS
175	174	5	9	7.8	10707	PASS
176	174	95	101	98.3	135033	PASS
177	176	5	9	6.7	8996	PASS