


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF042319\  
 Data File : VF062256.D  
 Acq On : 23 Apr 2019 9:22  
 Operator : FY/SY  
 Sample : BFB  
 Misc : 5.00µ/5mL/MSVOA F/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_F  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82F041719S.M  
 Title : SW846 8260  
 Last Update : Fri Apr 19 23:52:01 2019

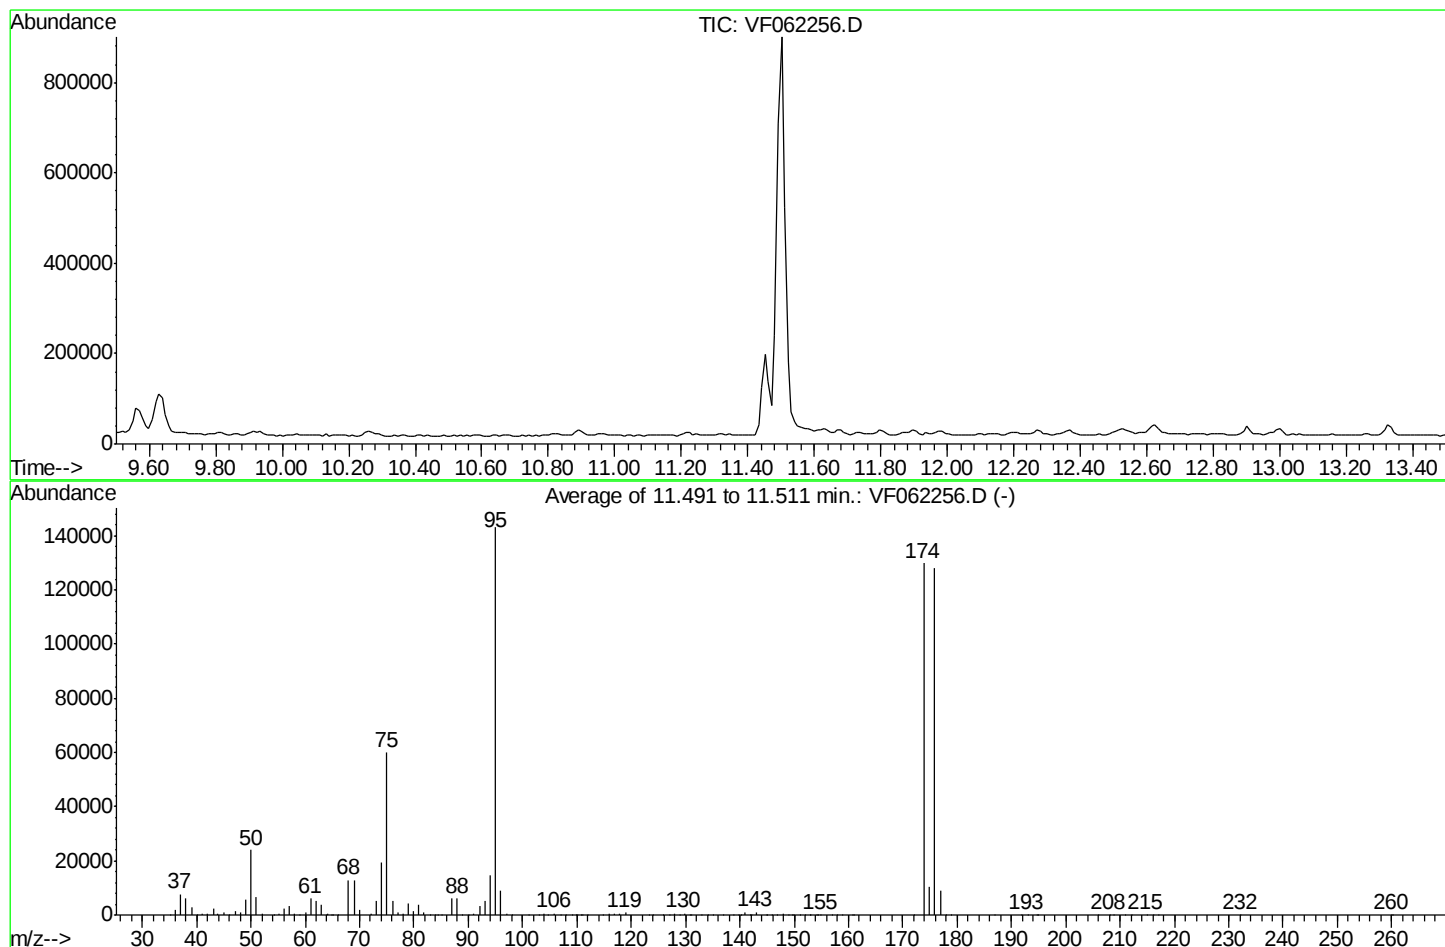

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1103

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.8      | 23996   | PASS             |
| 75          | 95           | 30           | 60           | 41.8      | 59872   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 143160  | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 9010    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 90.7      | 129794  | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 10350   | PASS             |
| 176         | 174          | 95           | 101          | 98.6      | 127946  | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 8804    | PASS             |