


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF042419\
 Data File : VF062276.D
 Acq On : 24 Apr 2019 12:06
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F042419S.M
 Title : SW846 8260
 Last Update : Thu Apr 25 08:40:59 2019

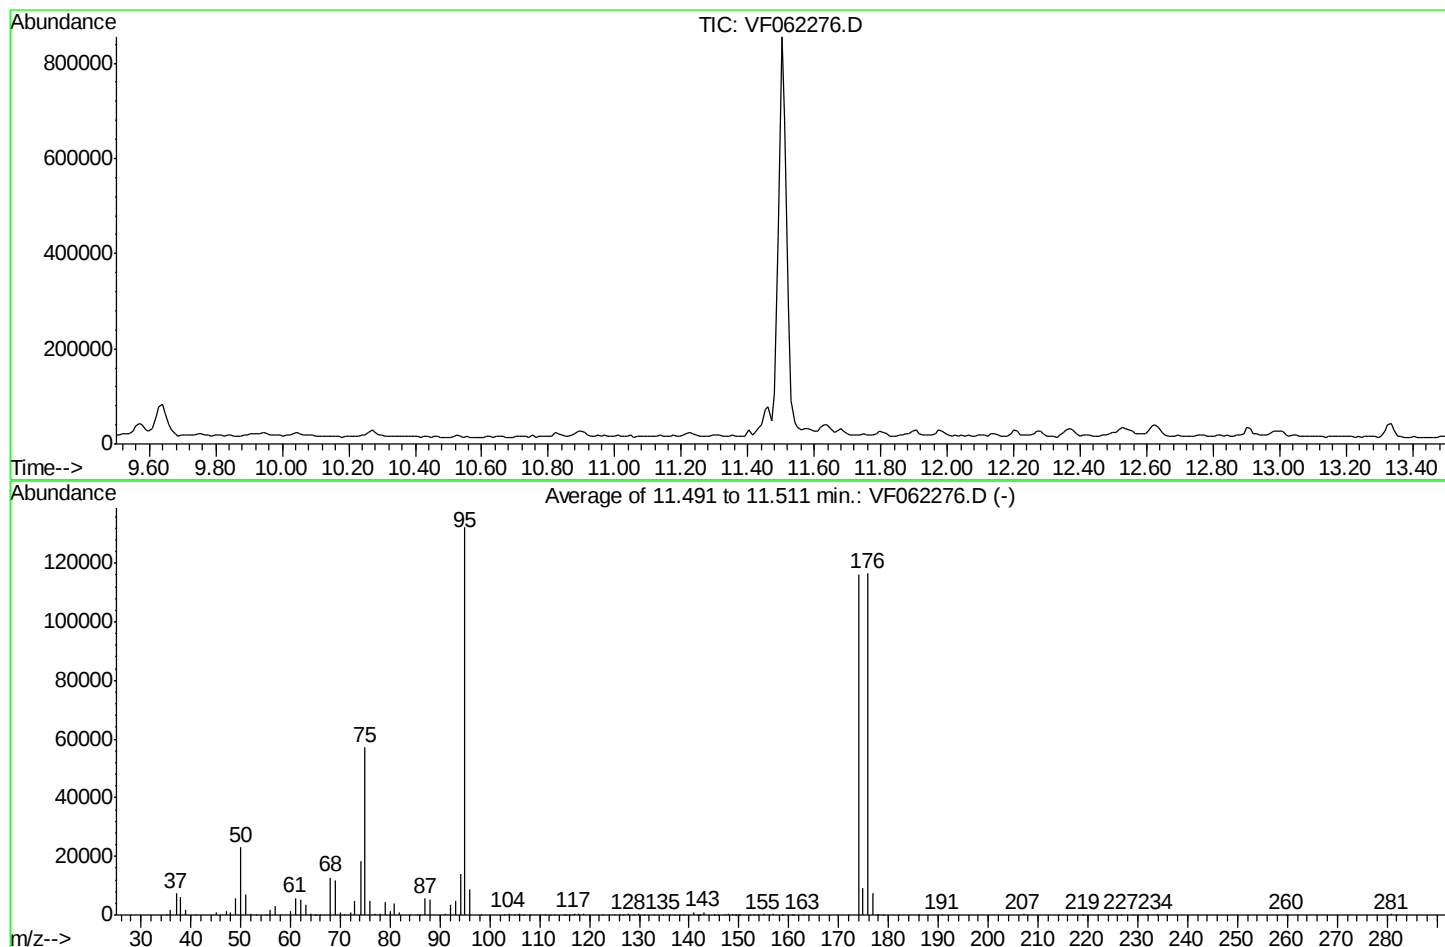

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	23126	PASS
75	95	30	60	43.1	57008	PASS
95	95	100	100	100.0	132229	PASS
96	95	5	9	6.7	8924	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.9	116194	PASS
175	174	5	9	7.8	9028	PASS
176	174	95	101	100.2	116482	PASS
177	176	5	9	6.4	7488	PASS