


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF042519\  
Data File : VF062287.D  
Acq On : 25 Apr 2019 12:04  
Operator : FY/SY  
Sample : BFB  
Misc : 5.00µ/5mL/MSVOA F/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_F  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82F042419S.M  
Title : SW846 8260  
Last Update : Thu Apr 25 08:40:59 2019

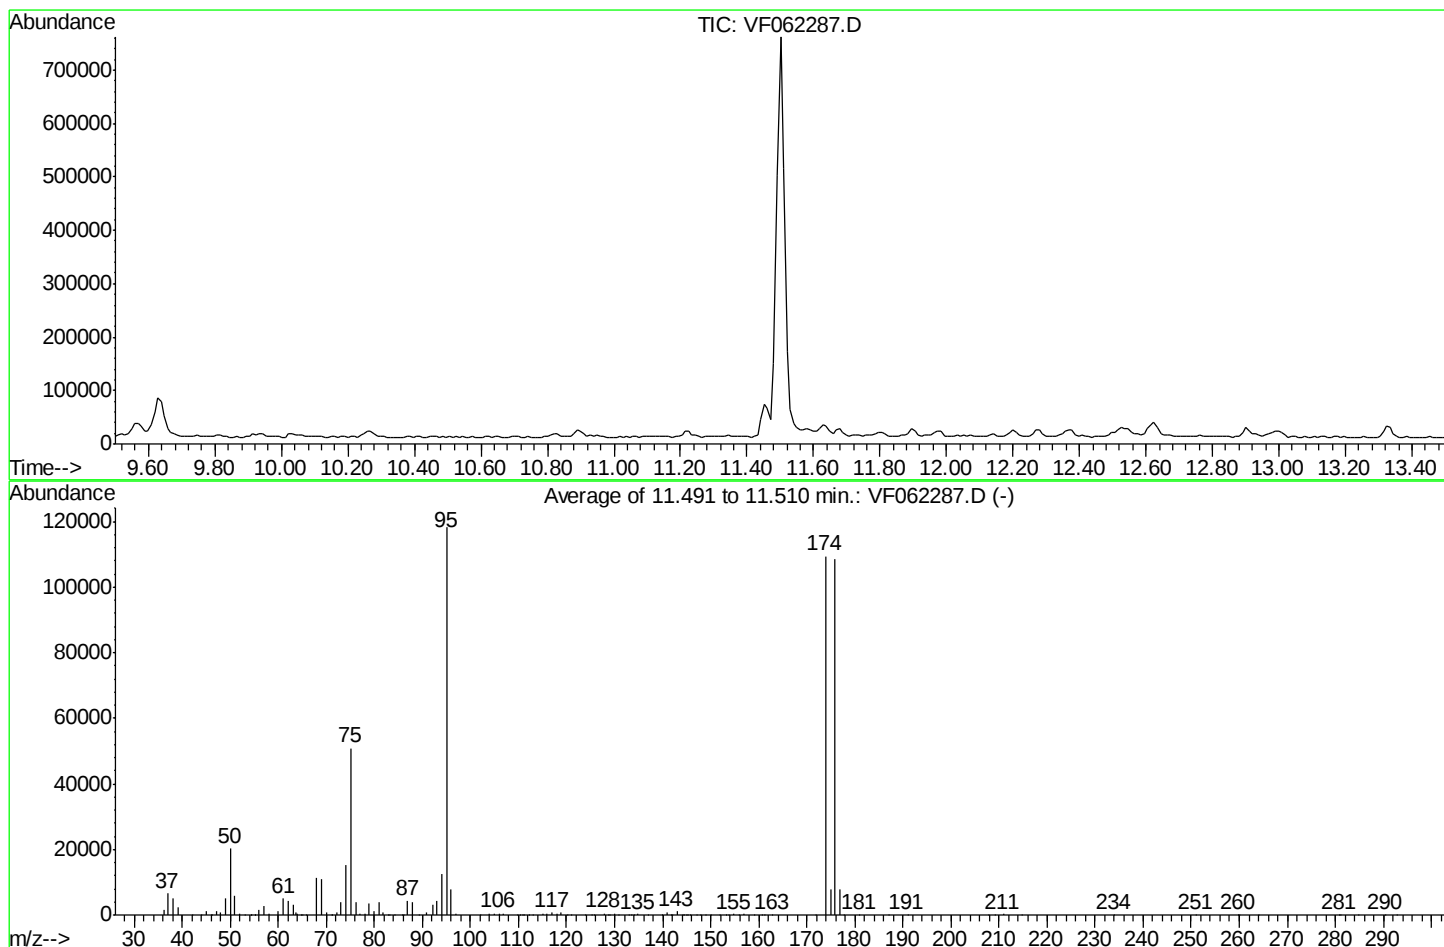

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.1      | 20246   | PASS             |
| 75          | 95           | 30           | 60           | 43.0      | 50845   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 118229  | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 7716    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 92.6      | 109504  | PASS             |
| 175         | 174          | 5            | 9            | 7.3       | 7956    | PASS             |
| 176         | 174          | 95           | 101          | 99.1      | 108553  | PASS             |
| 177         | 176          | 5            | 9            | 7.3       | 7920    | PASS             |