


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF043019\
 Data File : VF062330.D
 Acq On : 30 Apr 2019 12:47
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F042419S.M
 Title : SW846 8260
 Last Update : Thu Apr 25 08:40:59 2019

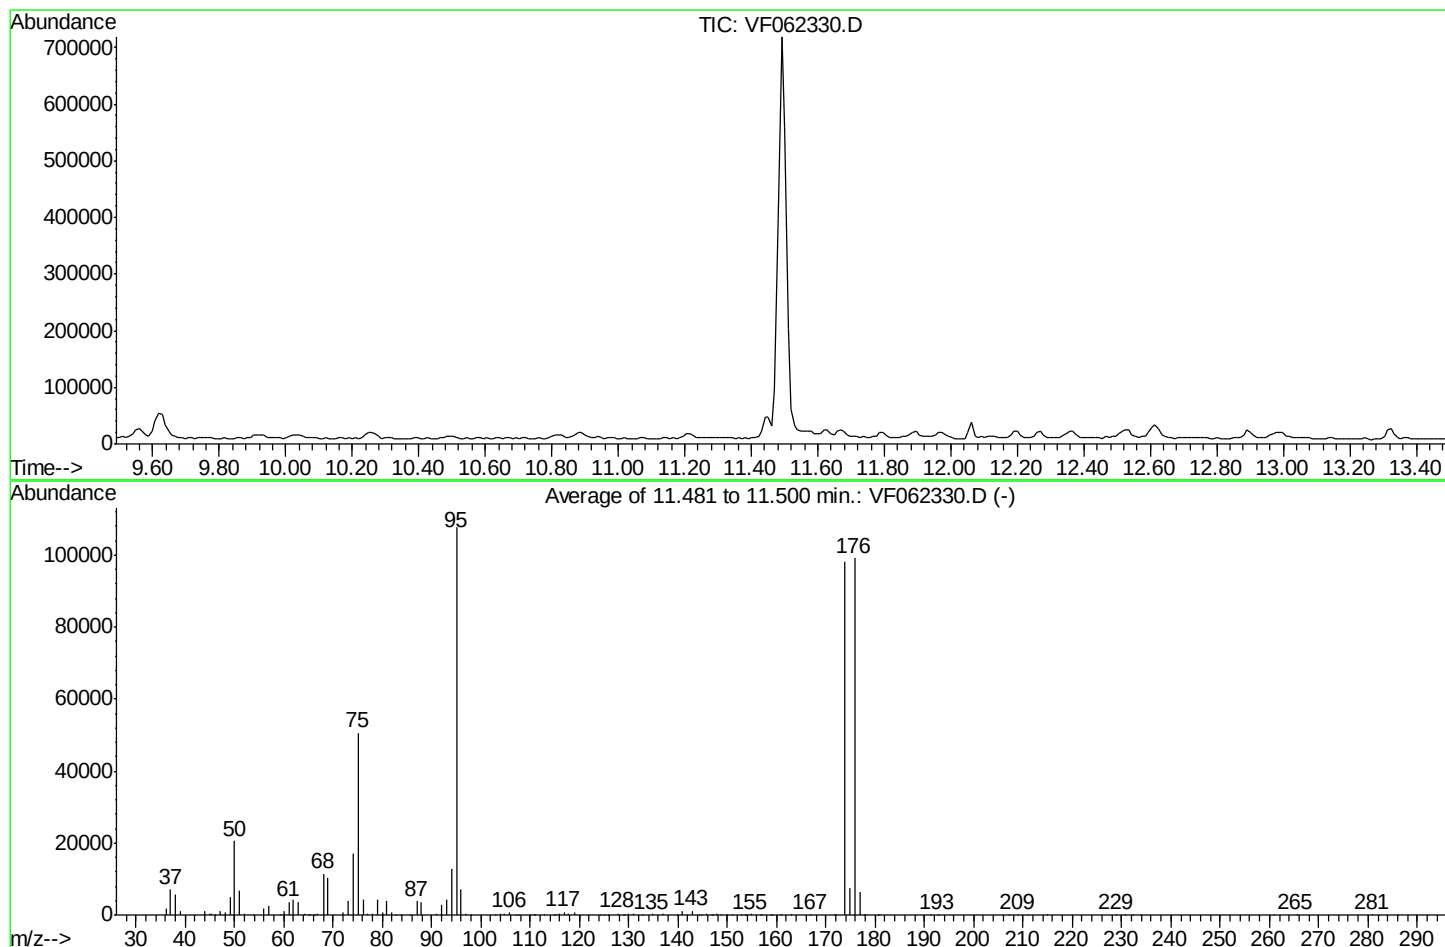

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	20597	PASS
75	95	30	60	46.9	50520	PASS
95	95	100	100	100.0	107728	PASS
96	95	5	9	6.5	6972	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.2	98229	PASS
175	174	5	9	7.5	7323	PASS
176	174	95	101	100.9	99080	PASS
177	176	5	9	6.3	6261	PASS