




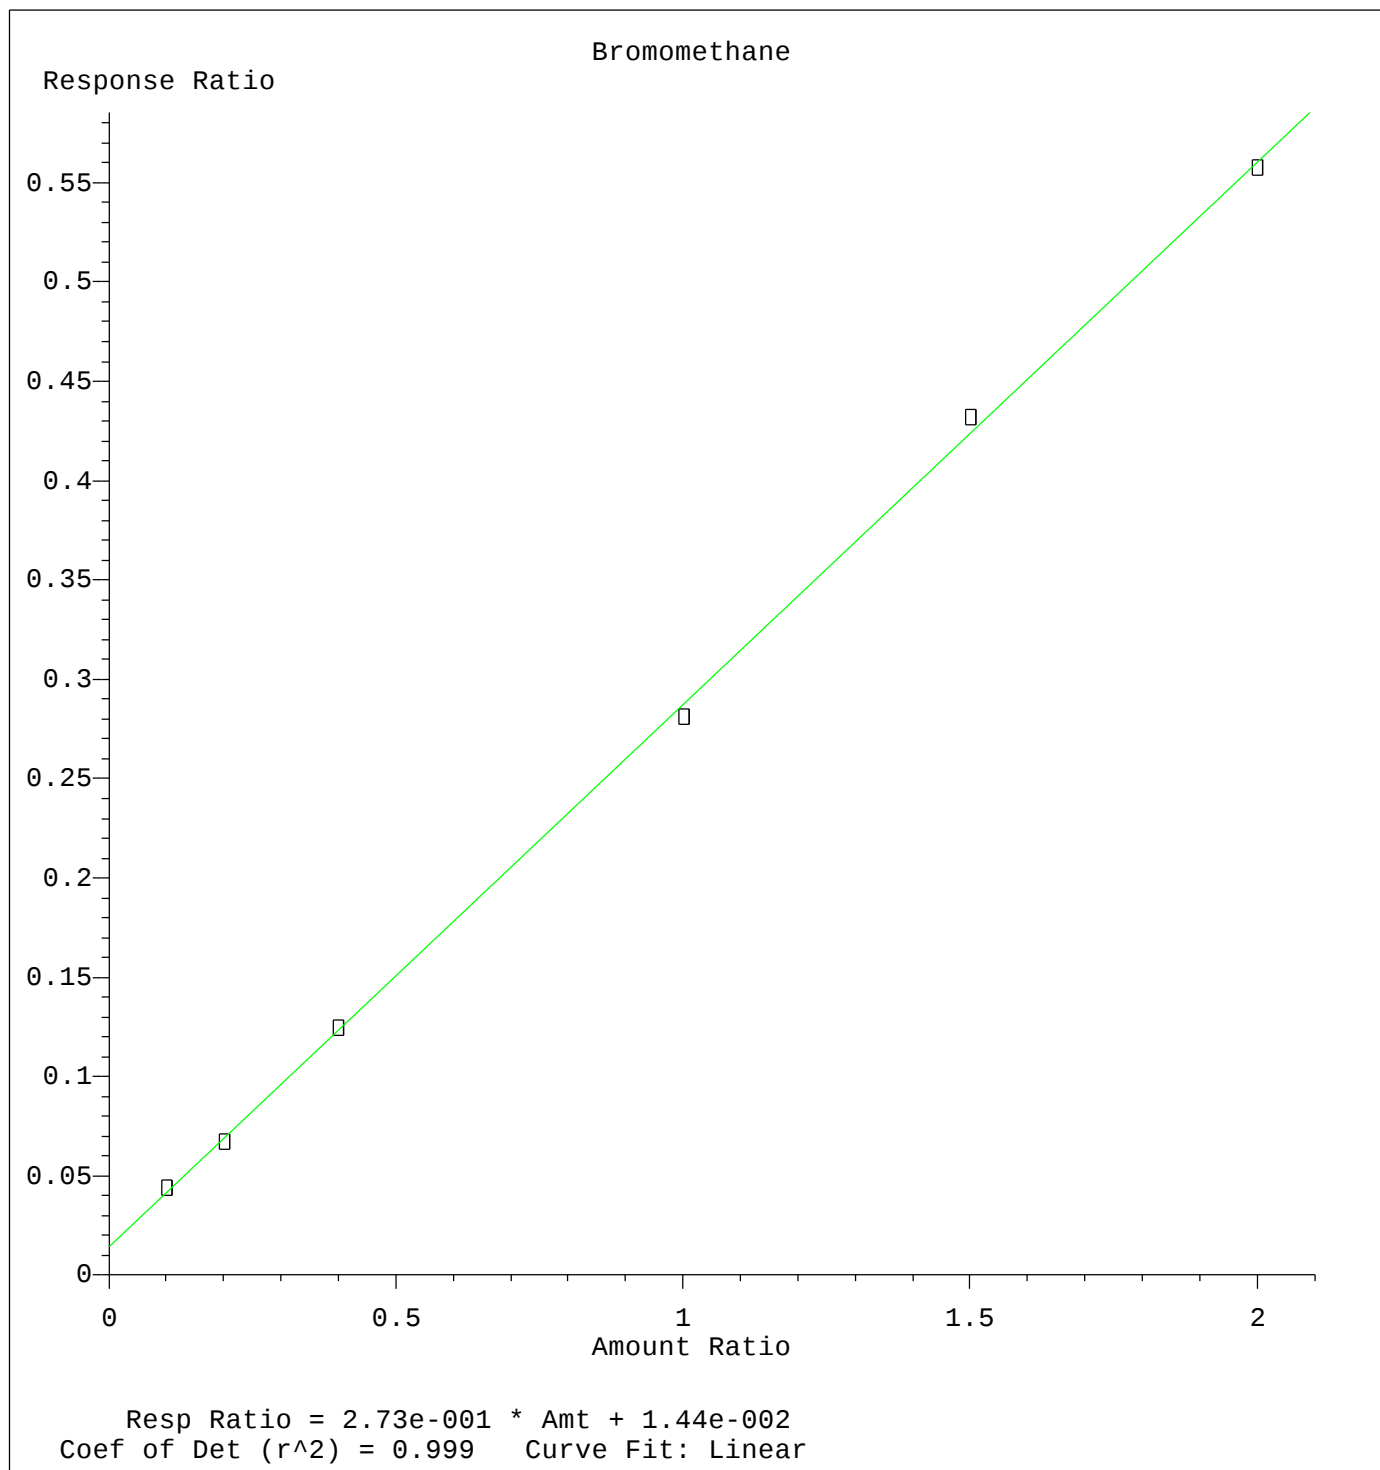


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Calibration Table Last Updated: Tue May 07 04:34:57 2019

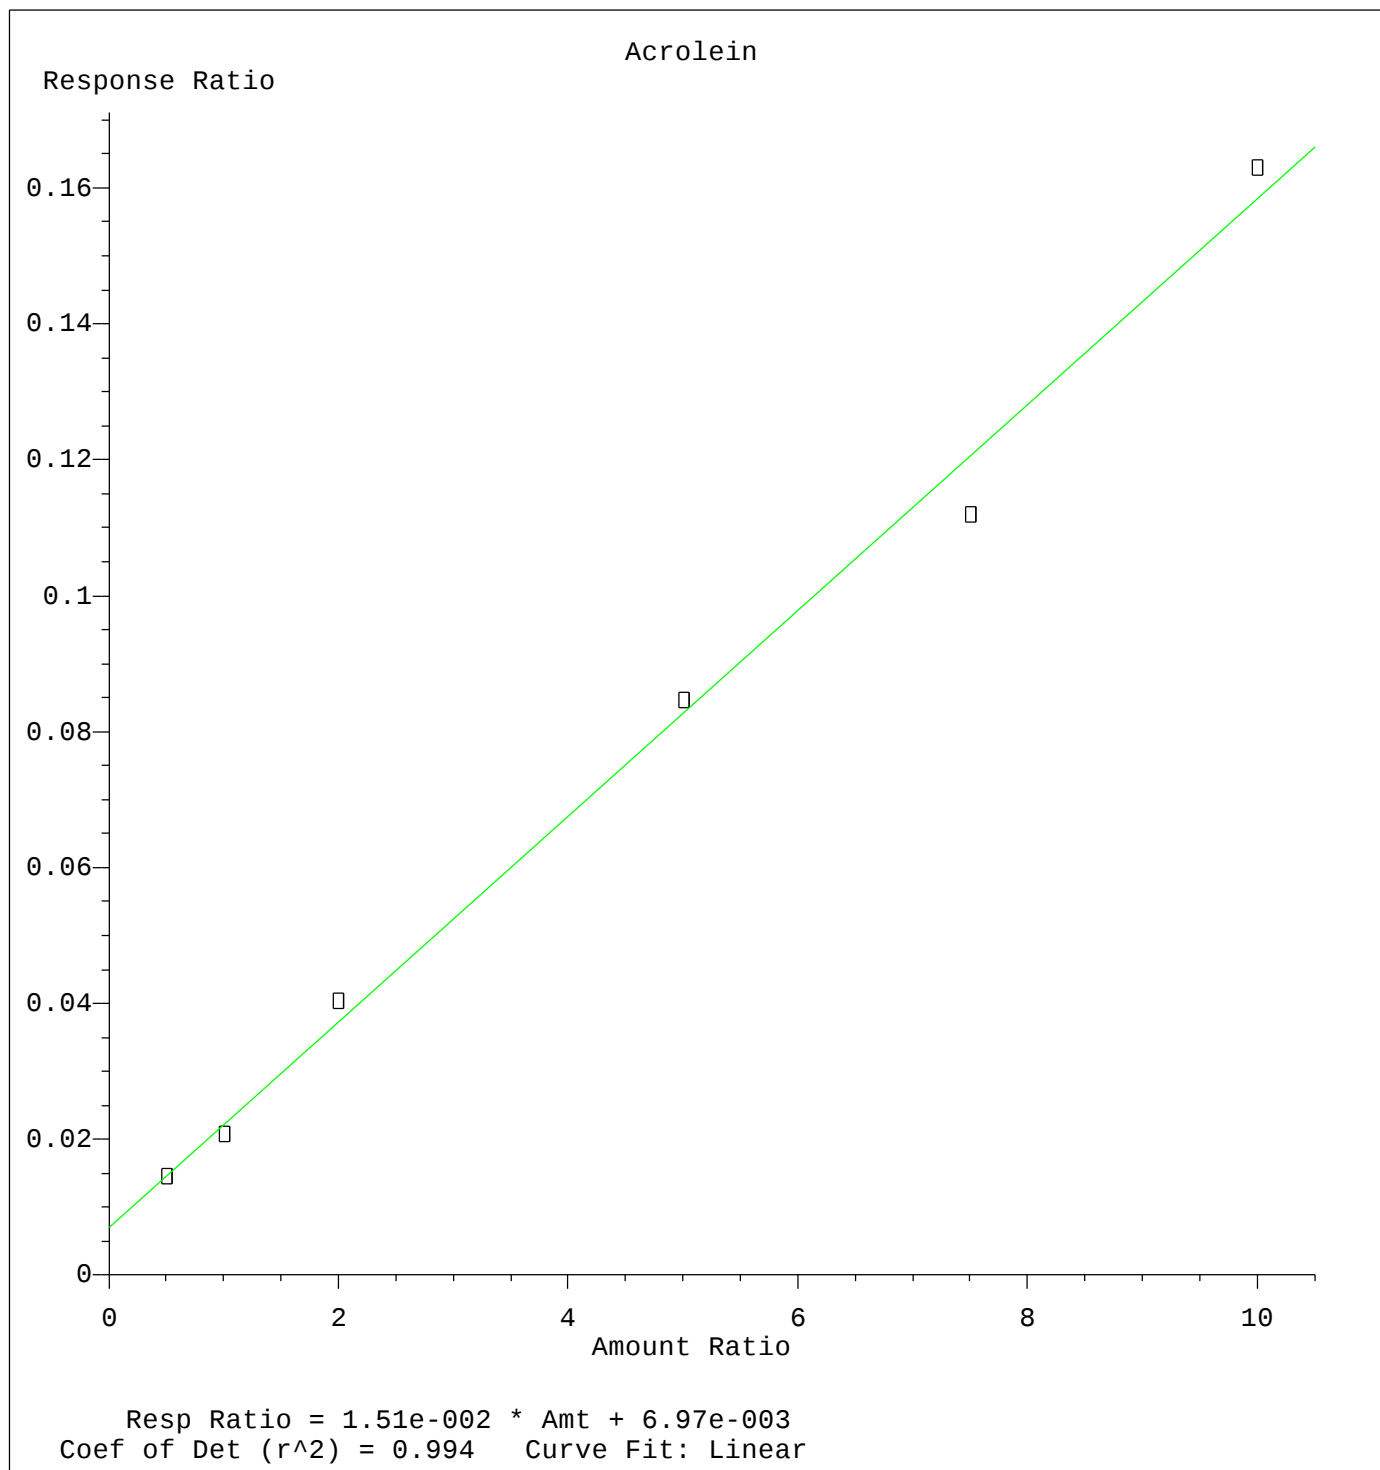


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Calibration Table Last Updated: Tue May 07 04:34:57 2019

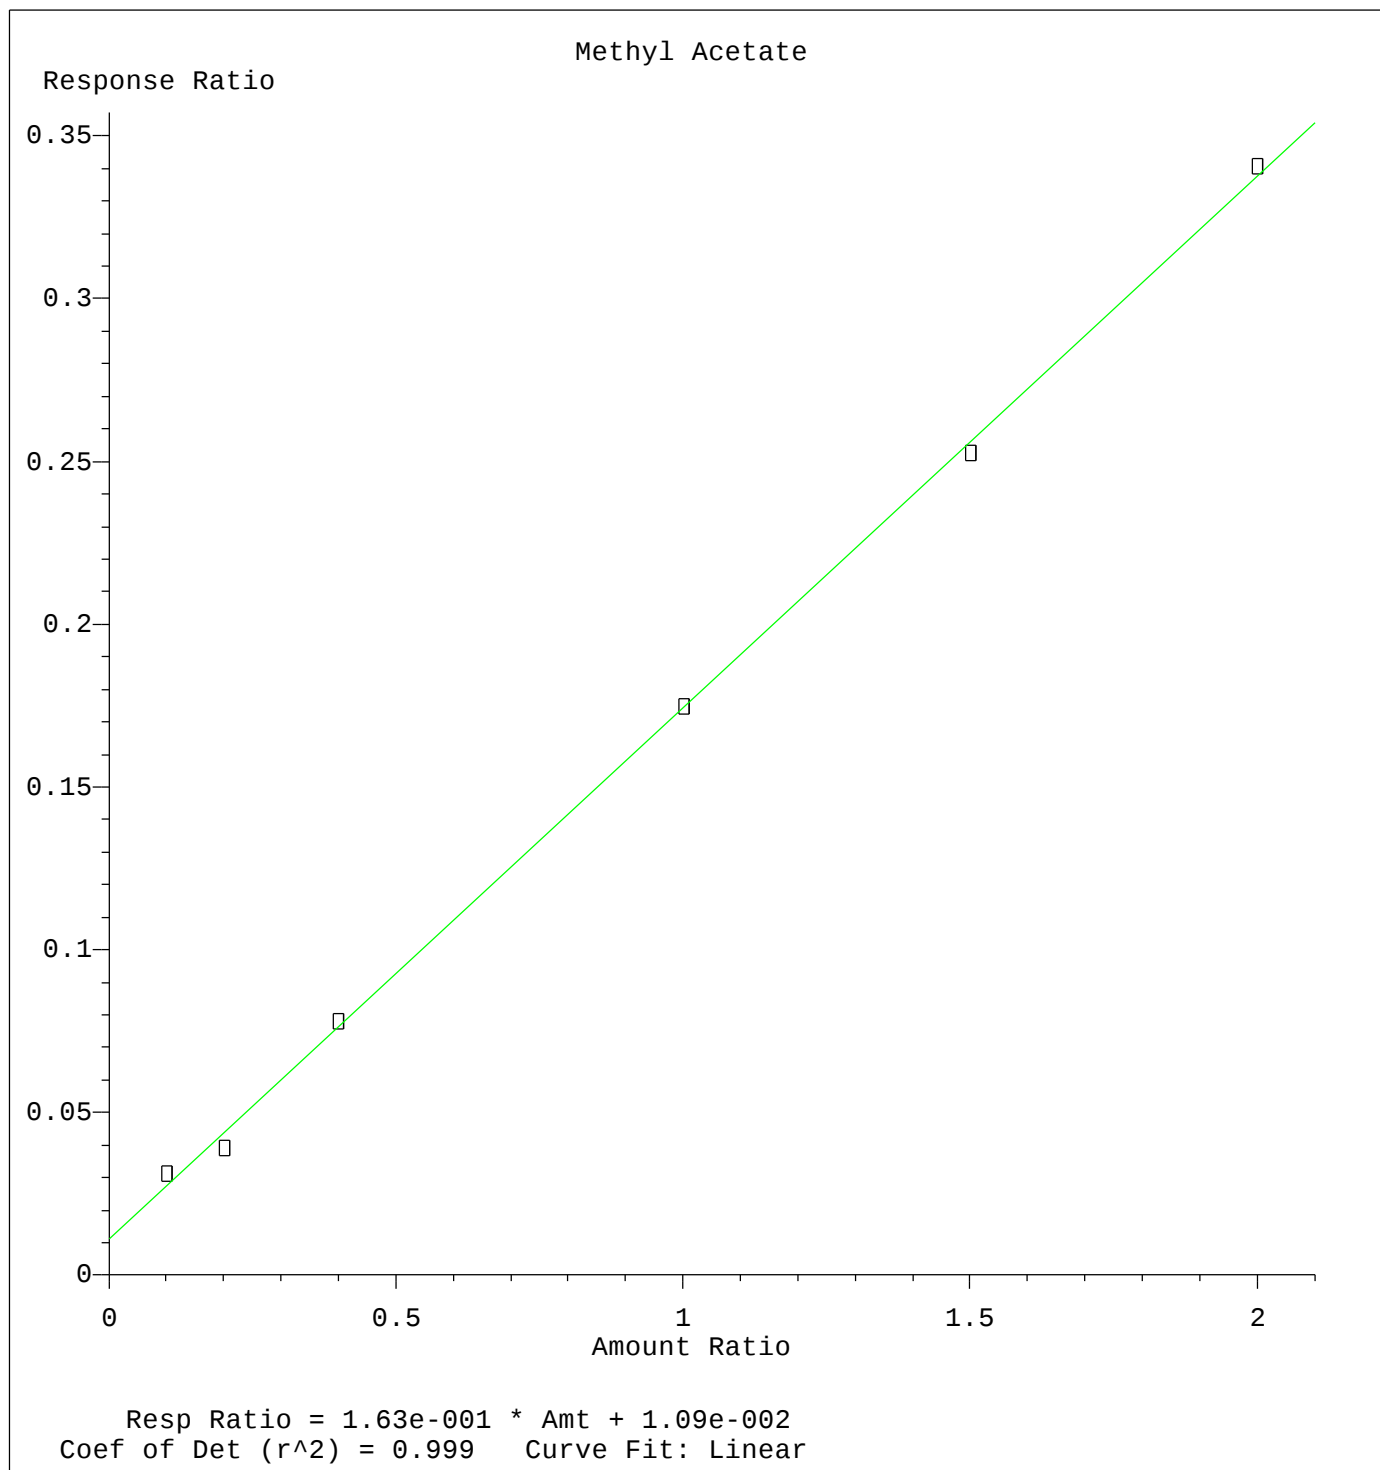


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Calibration Table Last Updated: Tue May 07 04:34:57 2019

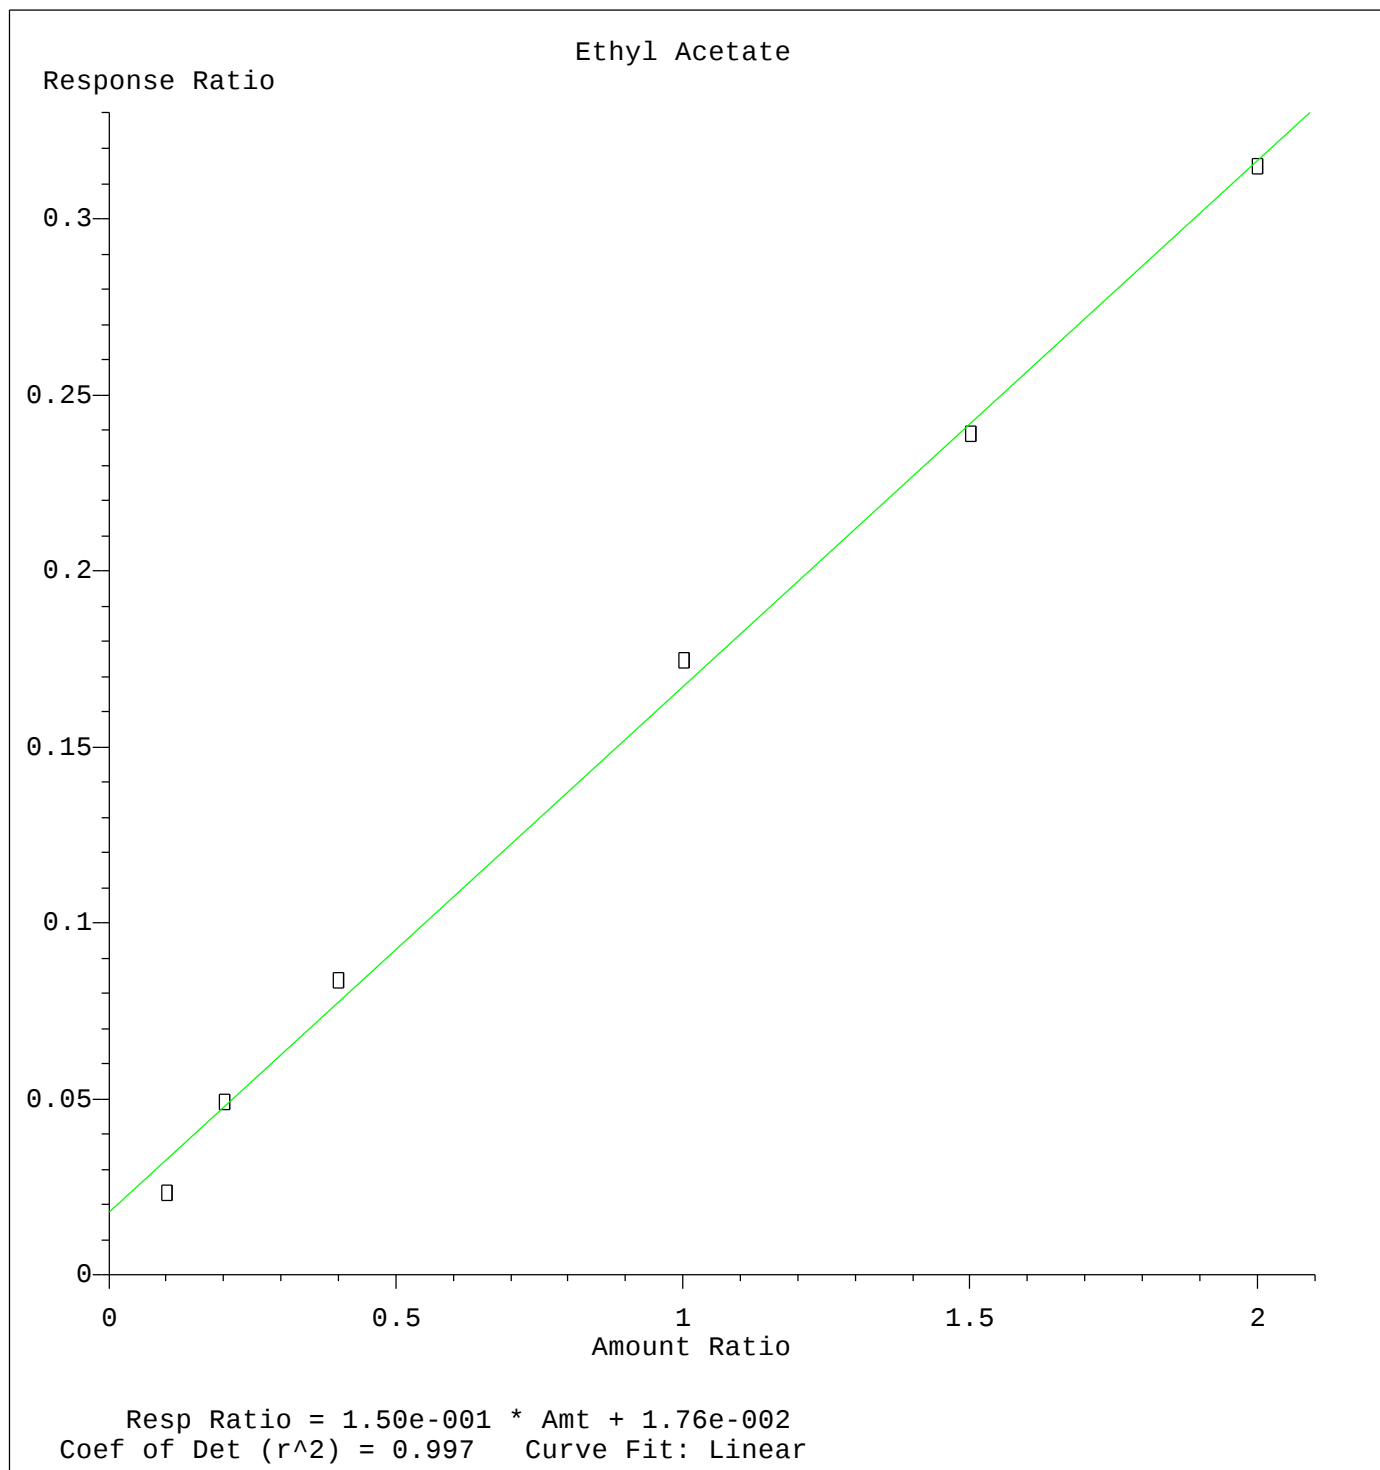

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Calibration Table Last Updated: Tue May 07 04:34:57 2019

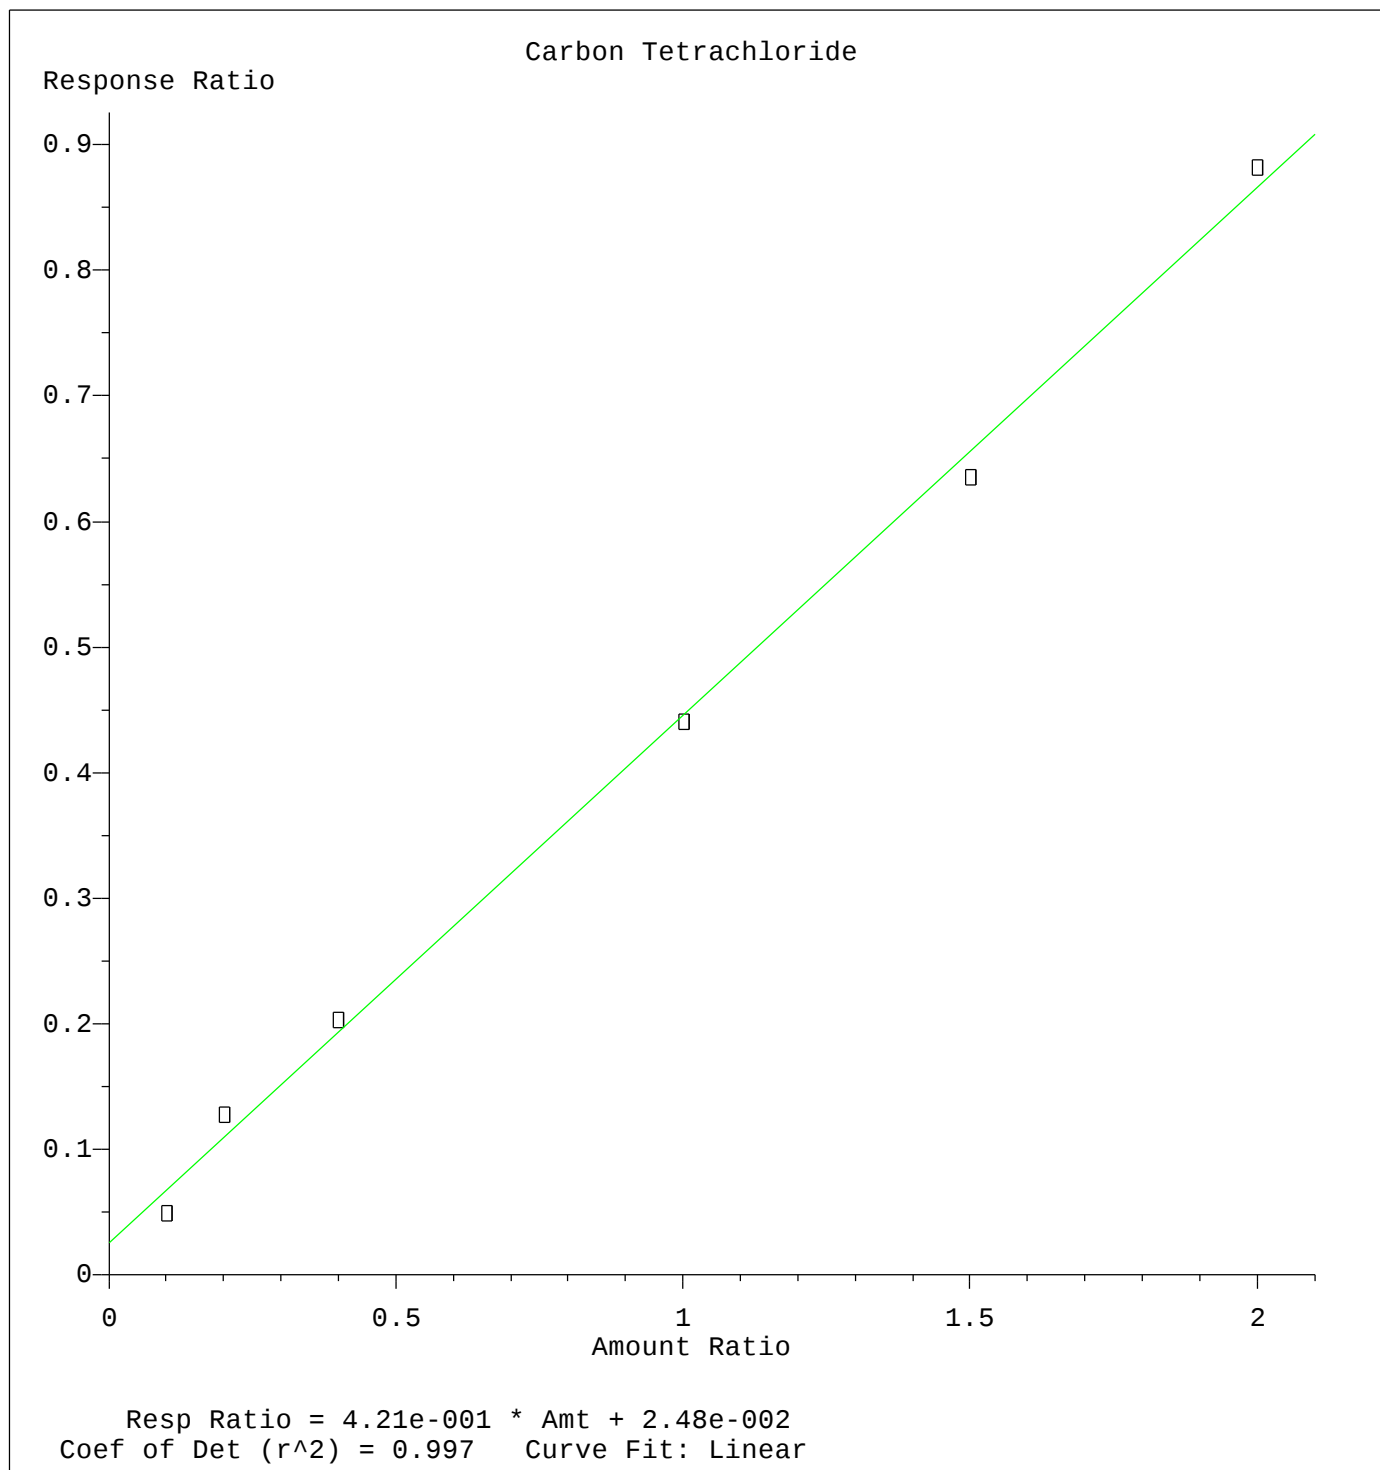

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Calibration Table Last Updated: Tue May 07 04:34:57 2019

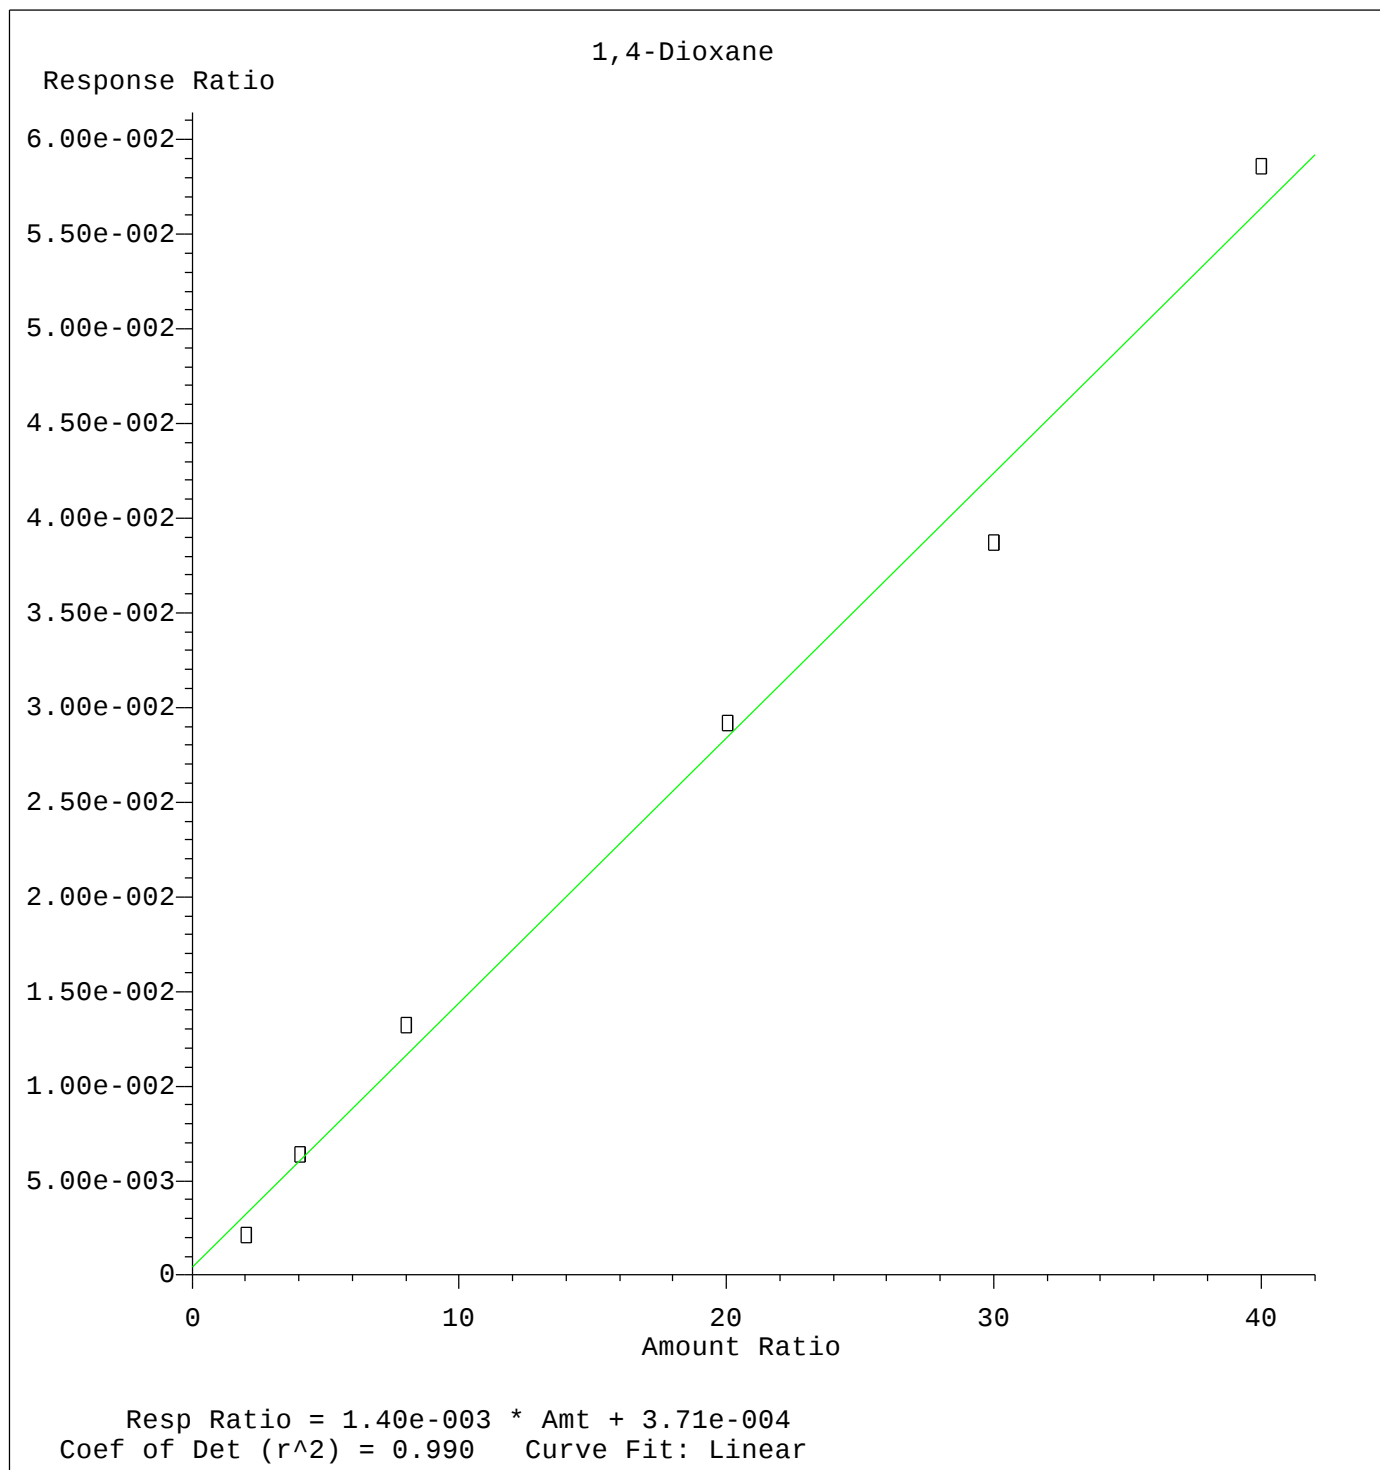

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Calibration Table Last Updated: Tue May 07 04:34:57 2019