


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF050819\
 Data File : VF062370.D
 Acq On : 8 May 2019 10:27
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Title : SW846 8260
 Last Update : Tue May 07 04:34:57 2019

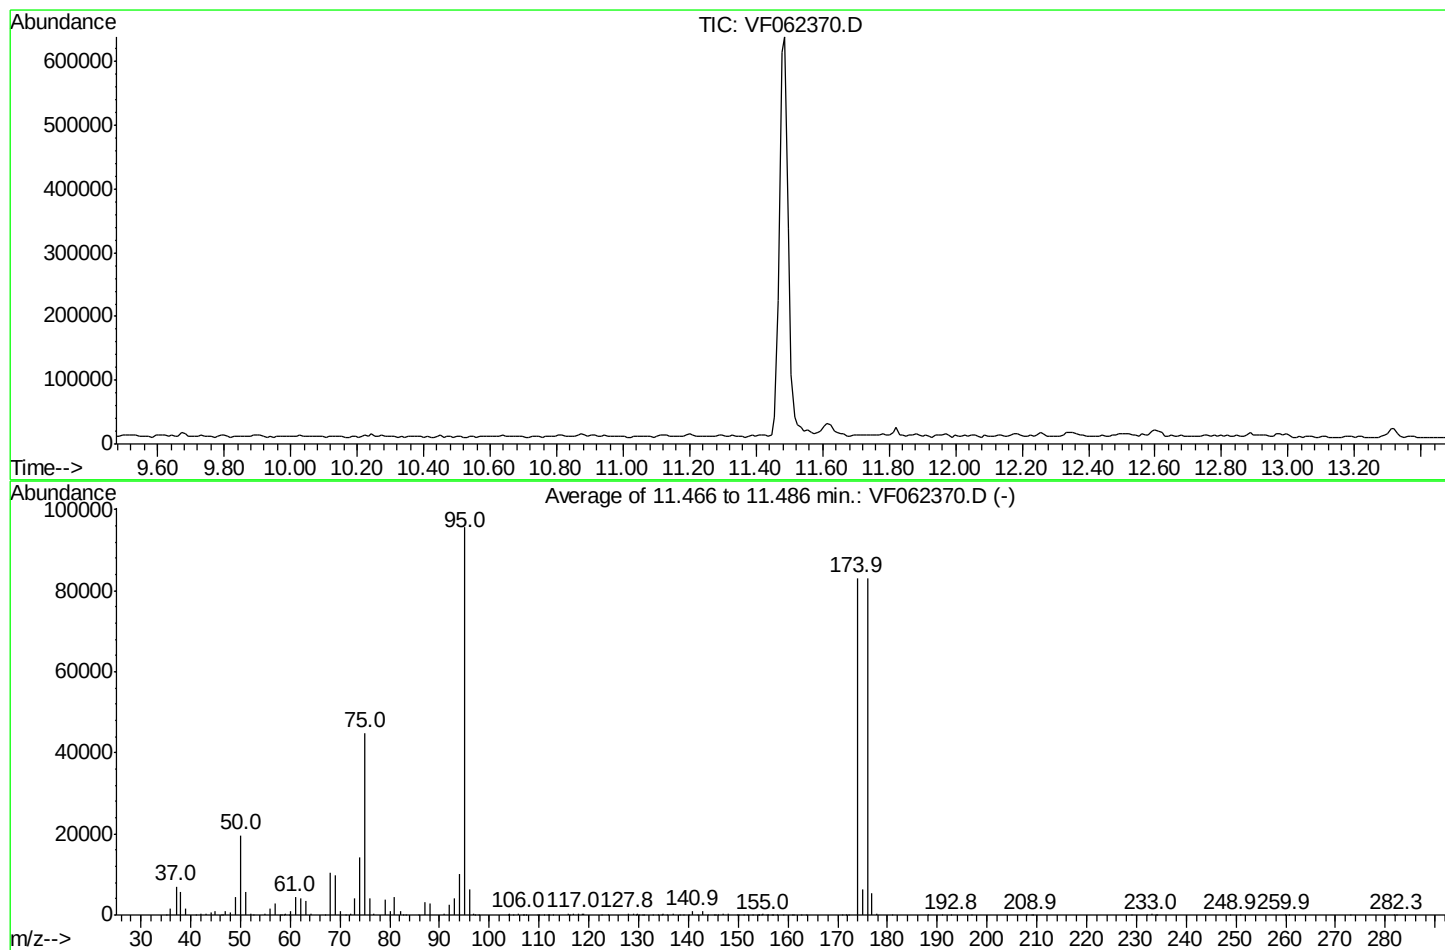

AutoFind: Scans 1109, 1110, 1111; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	19628	PASS
75	95	30	60	47.0	44962	PASS
95	95	100	100	100.0	95621	PASS
96	95	5	9	6.5	6213	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.9	83096	PASS
175	174	5	9	7.6	6332	PASS
176	174	95	101	100.0	83096	PASS
177	176	5	9	6.5	5364	PASS