

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF051019\
 Data File : VF062424.D
 Acq On : 10 May 2019 15:35
 Operator : FY/SY
 Sample : K2641-07RE
 Misc : 6.20g/5mL/MSVOA F/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 CL-02-050719-DRE

Manual Integrations
 APPROVED

MMDadoda
 5/11/2019 3:55:36 PM

Quant Time: May 10 16:02:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 07 04:34:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.06	168	383779	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.78	114	540645	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.92	117	388601	50.00	ug/l	0.02
72) 1,4-Dichlorobenzene-d4	12.62	152	210213	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.04	65	208788	57.57	ug/l	0.02
Spiked Amount 50.000			Recovery	=	115.14%	
35) Dibromofluoromethane	4.31	113	242601	56.32	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.64%	
50) Toluene-d8	7.72	98	455090	43.65	ug/l	0.02
Spiked Amount 50.000			Recovery	=	87.30%	
62) 4-Bromofluorobenzene	11.50	95	204221	43.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	86.82%	
Target Compounds						
16) Acetone	2.35	43	40492	55.190	ug/l	96
20) Methylene Chloride	2.35	84	20582m	7.754	ug/l	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF051019\
Data File : VF062424.D
Acq On : 10 May 2019 15:35
Operator : FY/SY
Sample : K2641-07RE
Misc : 6.20g/5mL/MSVOA F/SOIL
ALS Vial : 12 Sample Multiplier: 1


Instrument :
MSVOA_F
ClientSampleId :
CL-02-050719-DRE

Manual Integrations
APPROVED

MMDadoda
5/11/2019 3:55:36 PM

Quant Time: May 10 16:02:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Quant Title : SW846 8260
QLast Update : Tue May 07 04:34:57 2019
Response via : Initial Calibration

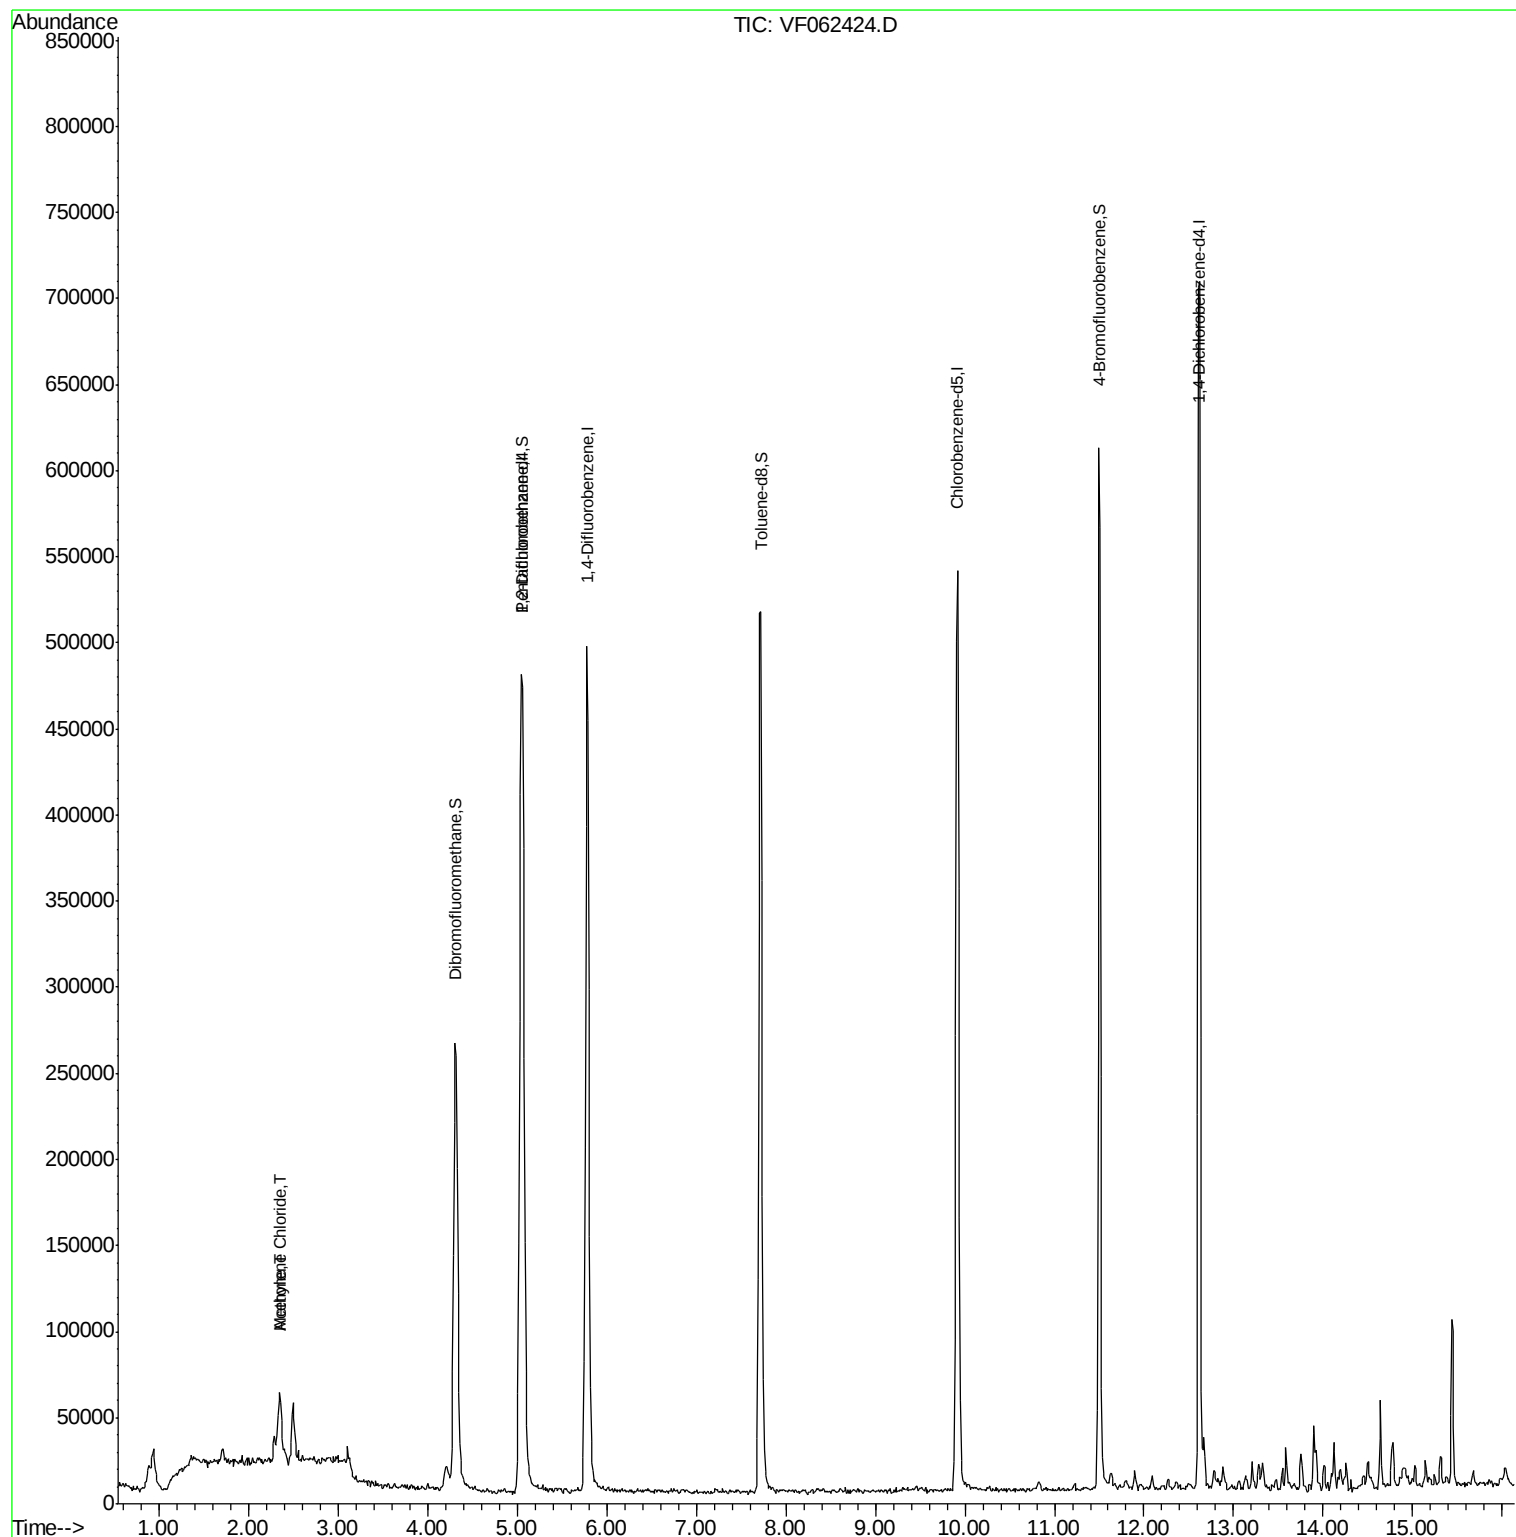

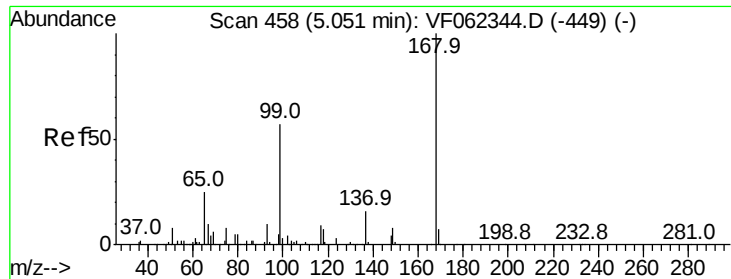

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.06 min Scan# 459

Delta R.T. 0.01 min

Lab File: VF062424.D

Acq: 10 May 2019 15:35

Instrument :

MSVOA_F

ClientSampleId :

CL-02-050719-DRE

Tot Ion:168 Resp: 383779

Ion Ratio Lower Upper

168 100


99 58.1 45.9 68.9

Manual Integrations

APPROVED

MMDadoda

5/11/2019 3:55:36 PM

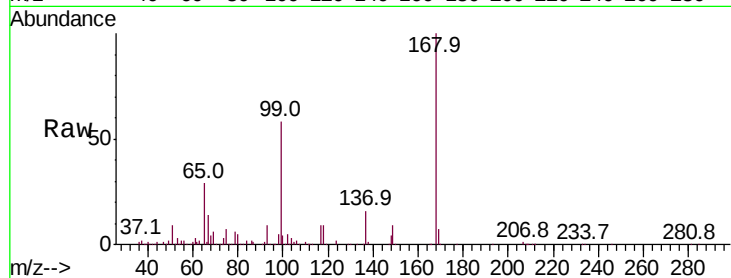

Abundance Ion 167.90 (167.60 to 168.60): VF0

Ion 98.90 (98.60 to 99.60): VF0

5.06

150000



100000

50000

0

4.90 5.00 5.10 5.20 5.30

Time-->

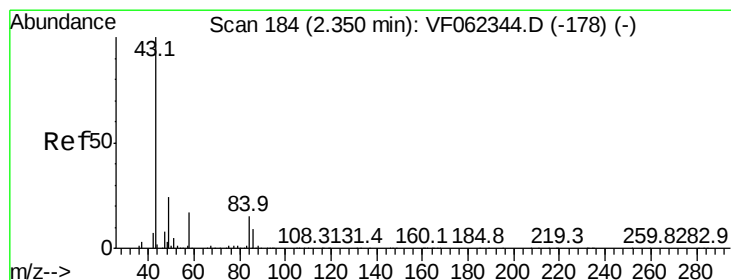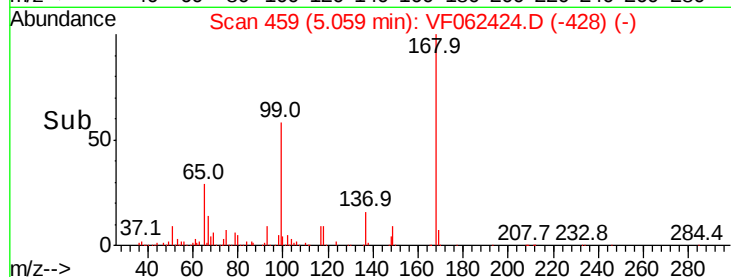

#16

Acetone

Concen: 55.190 ug/l

RT: 2.35 min Scan# 184

Delta R.T. -0.00 min

Lab File: VF062424.D


Acq: 10 May 2019 15:35

Tgt Ion: 43 Resp: 40492

Ion Ratio Lower Upper

43 100

58 14.8 13.1 19.7

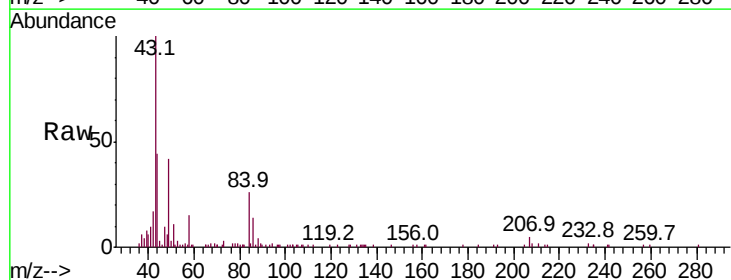

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0

2.35

15000


10000


5000

0

2.30 2.40

Time-->

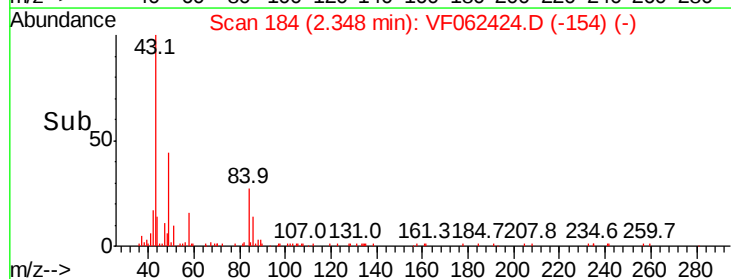

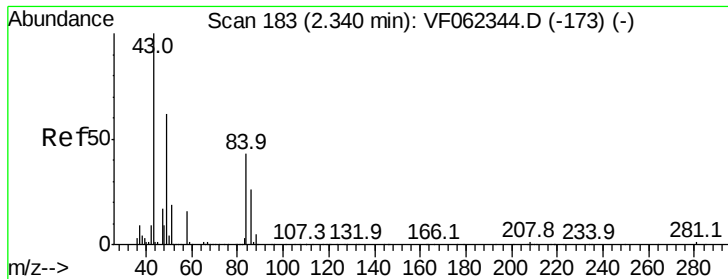





#20
Methvlene Chloride
Concen: 7.754 ug/l m
RT: 2.35 min Scan# 184
Delta R.T. 0.01 min
Lab File: VF062424.D
Acq: 10 May 2019 15:35

Instrument :
MSVOA_F
ClientSampleId :
CL-02-050719-DRE

Tot Ion	84	Resp	20582
Ion	Ratio	Lower	Upper
84	100		
49	159.5	117.5	176.3
51	42.7	37.0	55.4
86	55.4	49.3	73.9




Manual Integrations
APPROVED


MMDadoda
5/11/2019 3:55:36 PM

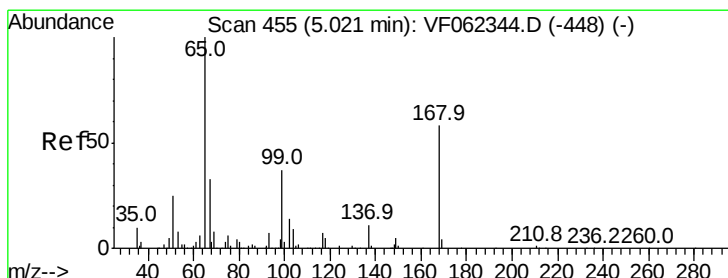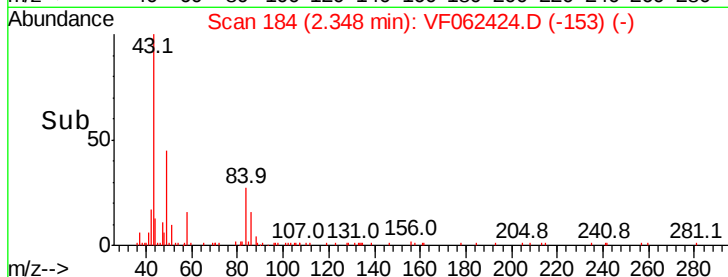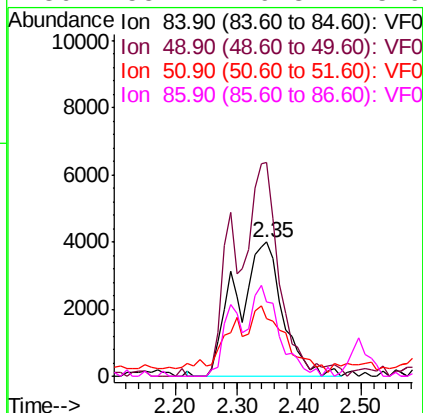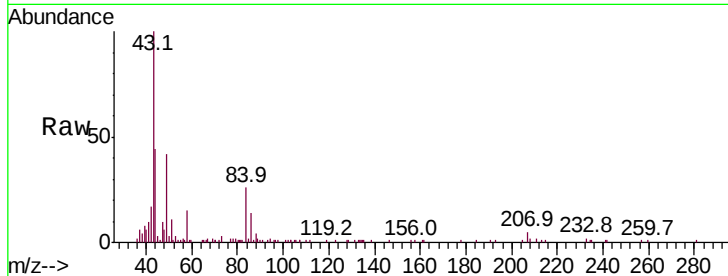

#33
1,2-Dichloroethane-d4
Concen: 57.567 ug/l
RT: 5.04 min Scan# 457
Delta R.T. 0.02 min
Lab File: VF062424.D
Acq: 10 May 2019 15:35

Tgt Ion	65	Resp	208788
Ion	Ratio	Lower	Upper
65	100		
67	45.0	0.0	85.8

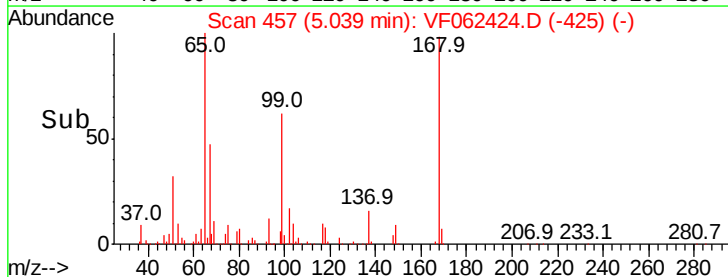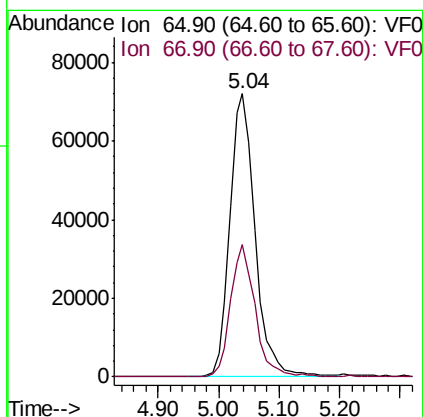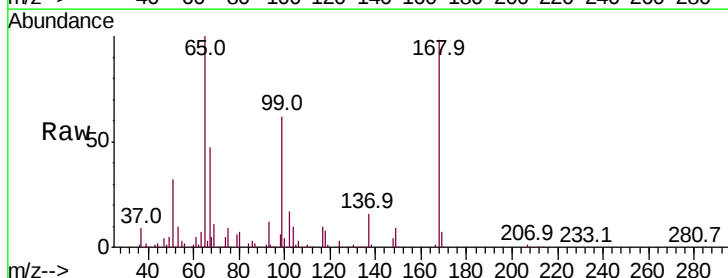

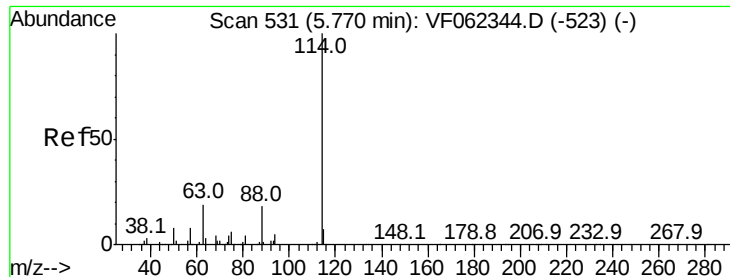

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.78 min Scan# 532

Delta R.T. 0.01 min

Lab File: VF062424.D

Acq: 10 May 2019 15:35

Instrument :

MSVOA_F





ClientSampleId :

CL-02-050719-DRE

Tot Ion:	114	Resp:	540645
Ion Ratio		Lower	Upper
114	100		
63	19.9	0.0	37.4
88	18.6	0.0	36.4

Manual Integrations
APPROVED

MMDadoda
5/11/2019 3:55:36 PM

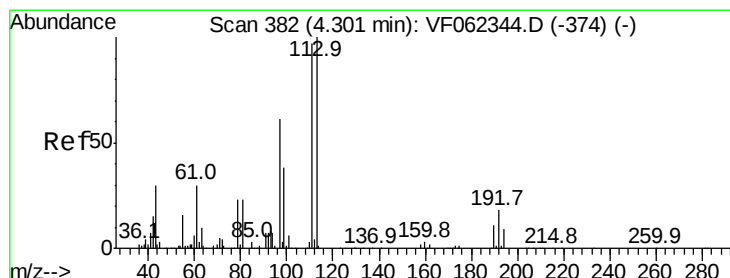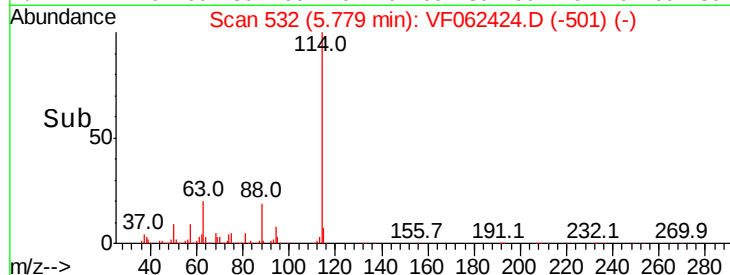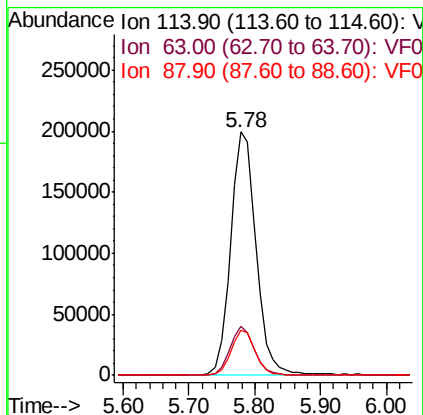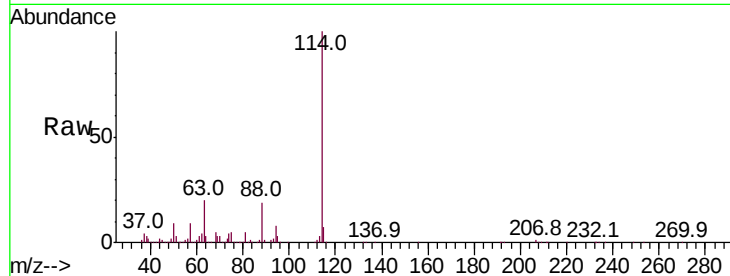

#35

Dibromofluoromethane

Concen: 56.324 ug/l




RT: 4.31 min Scan# 383


Delta R.T. 0.01 min

Lab File: VF062424.D

Acq: 10 May 2019 15:35

Tgt Ion:	113	Resp:	242601
Ion Ratio		Lower	Upper
113	100		
111	101.0	79.4	119.0
192	20.9	16.0	24.0

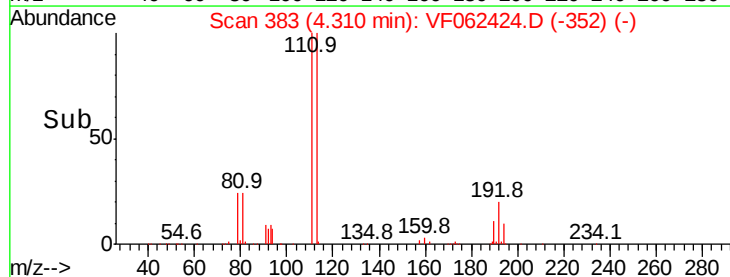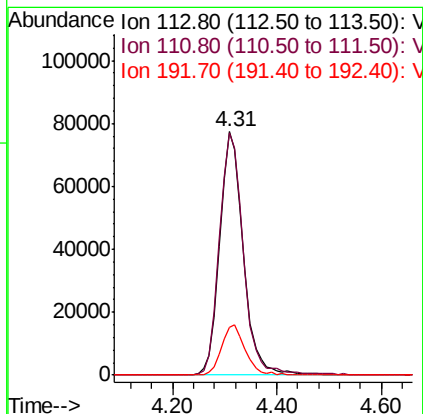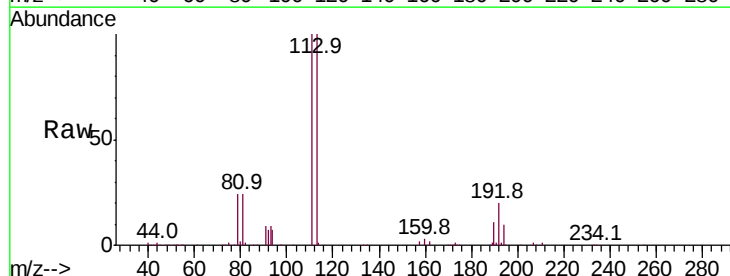

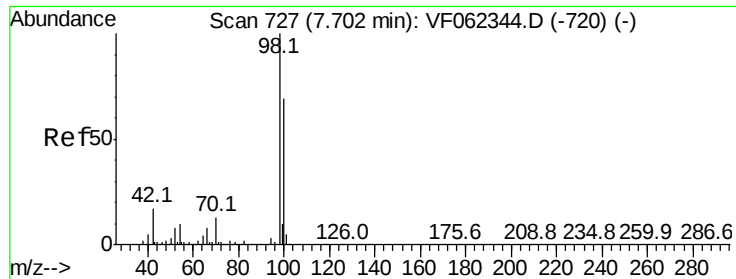





#50
Toluene-d8
Concen: 43.648 ug/l
RT: 7.72 min Scan# 729
Delta R.T. 0.02 min
Lab File: VF062424.D
Acq: 10 May 2019 15:35

Instrument :
MSVOA_F
ClientSampleId :
CL-02-050719-DRE

Tot Ion	Ratio	Lower	Upper
98	100		
100	68.0	53.3	79.9




Manual Integrations
APPROVED


MMDadoda
5/11/2019 3:55:36 PM

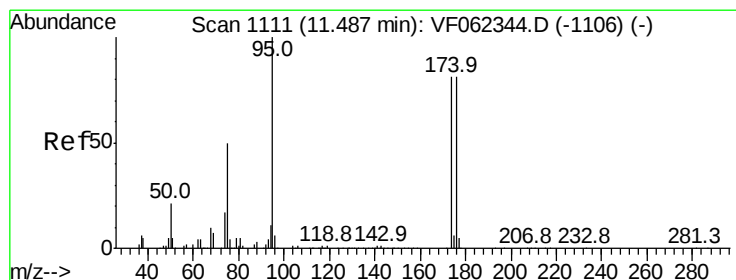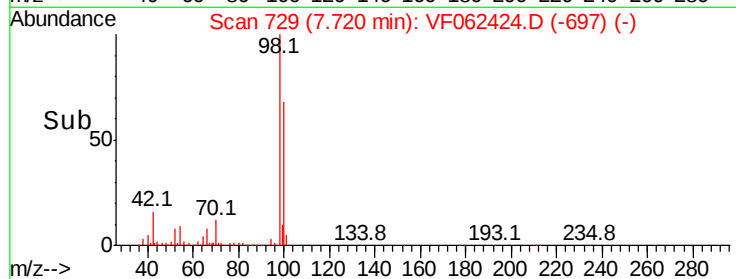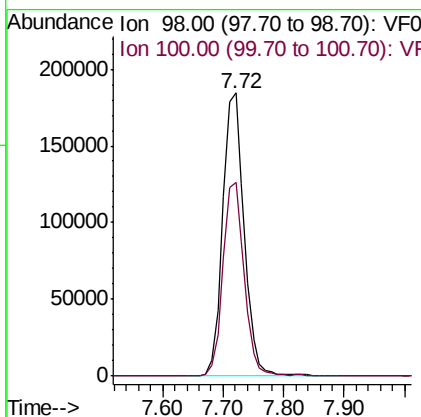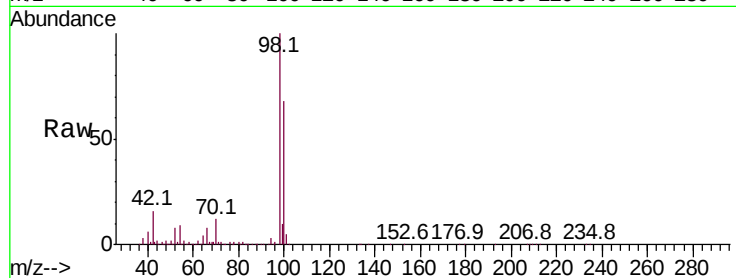

#62
4-Bromofluorobenzene
Concen: 43.415 ug/l
RT: 11.50 min Scan# 1112
Delta R.T. 0.01 min
Lab File: VF062424.D
Acq: 10 May 2019 15:35

Tgt Ion	Ratio	Lower	Upper
95	100		
174	98.1	0.0	191.8
176	97.0	0.0	193.2

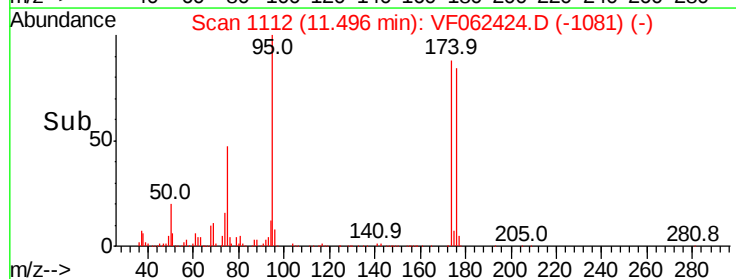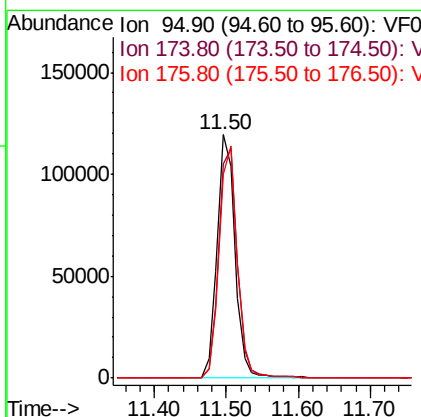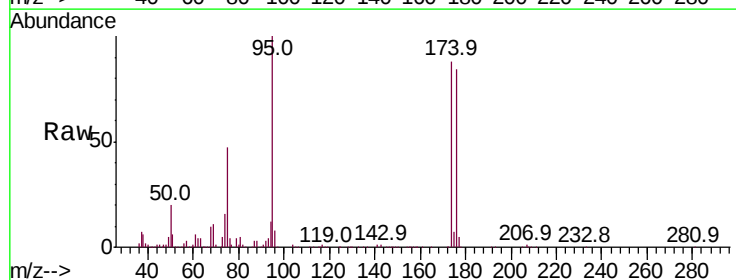

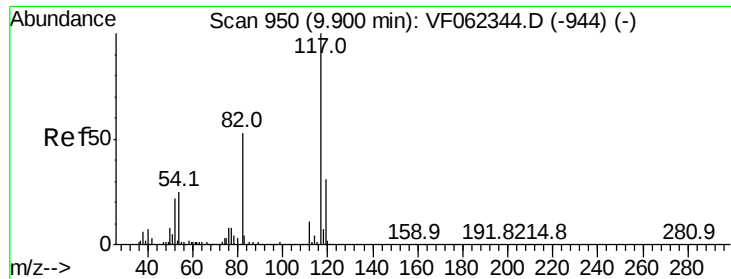





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.92 min Scan# 952
Delta R.T. 0.02 min
Lab File: VF062424.D
Acq: 10 May 2019 15:35

Instrument :
MSVOA_F
ClientSampleId :
CL-02-050719-DRE

Tot Ion	Ratio	Resp	Lower	Upper
117	100	388601		
82	52.3		42.2	63.2
119	33.7		25.0	37.4

Manual Integrations
APPROVED

MMDadoda
5/11/2019 3:55:36 PM

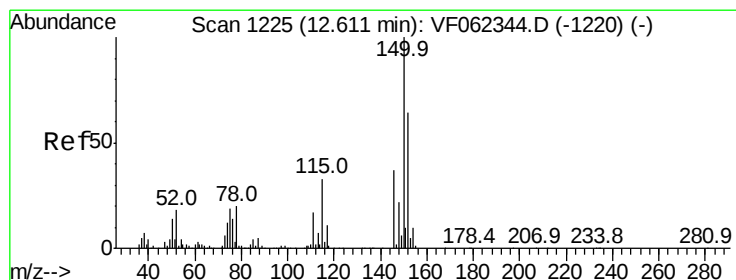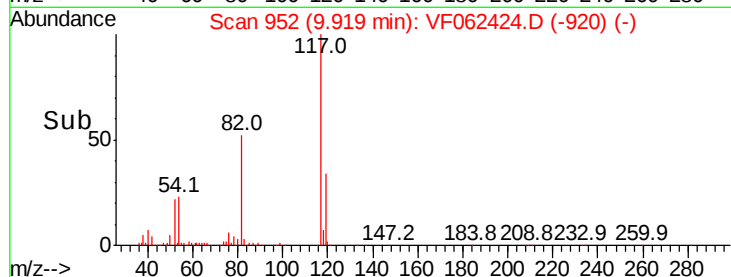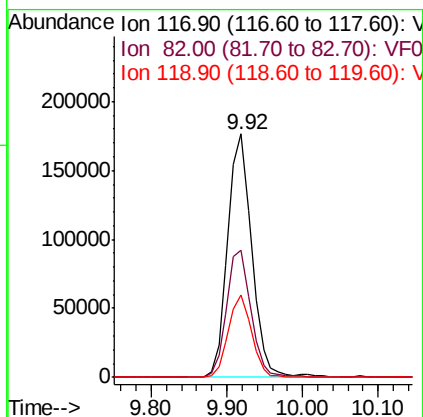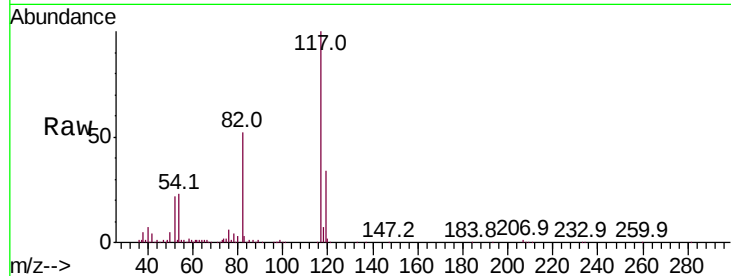

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.62 min Scan# 1226
Delta R.T. 0.01 min
Lab File: VF062424.D
Acq: 10 May 2019 15:35

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	210213		
115	52.9		26.4	79.2
150	147.5		0.0	335.0

