


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF051019\
 Data File : VF062432.D
 Acq On : 10 May 2019 20:15
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Title : SW846 8260
 Last Update : Tue May 07 04:34:57 2019

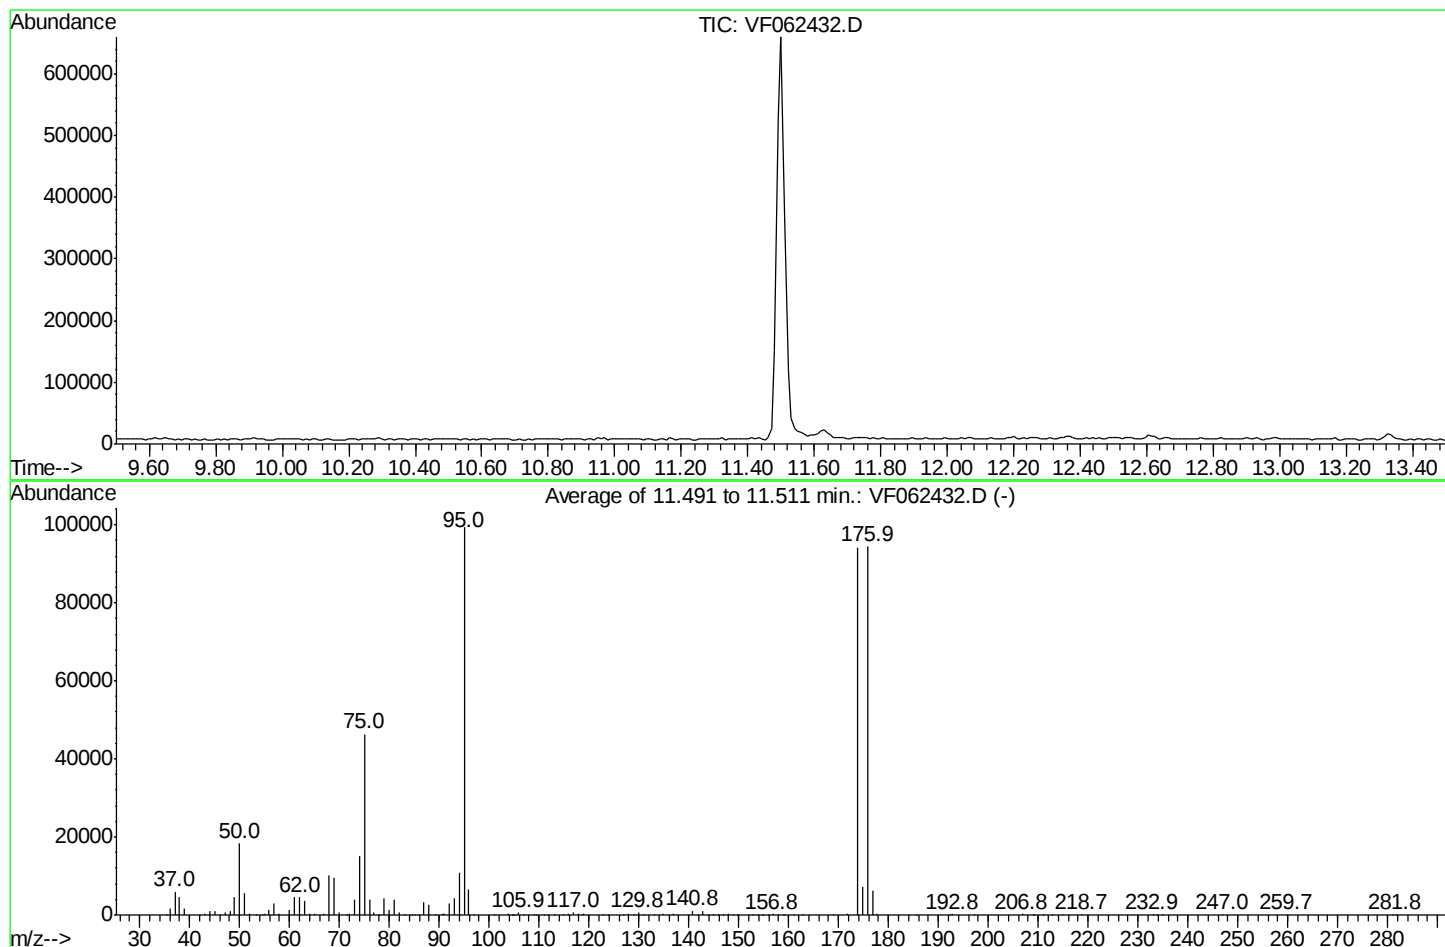

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	18273	PASS
75	95	30	60	46.6	46277	PASS
95	95	100	100	100.0	99333	PASS
96	95	5	9	6.5	6434	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	94.9	94221	PASS
175	174	5	9	7.5	7088	PASS
176	174	95	101	100.2	94418	PASS
177	176	5	9	6.5	6120	PASS