


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF051119\
 Data File : VF062451.D
 Acq On : 11 May 2019 9:21
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Title : SW846 8260
 Last Update : Tue May 07 04:34:57 2019

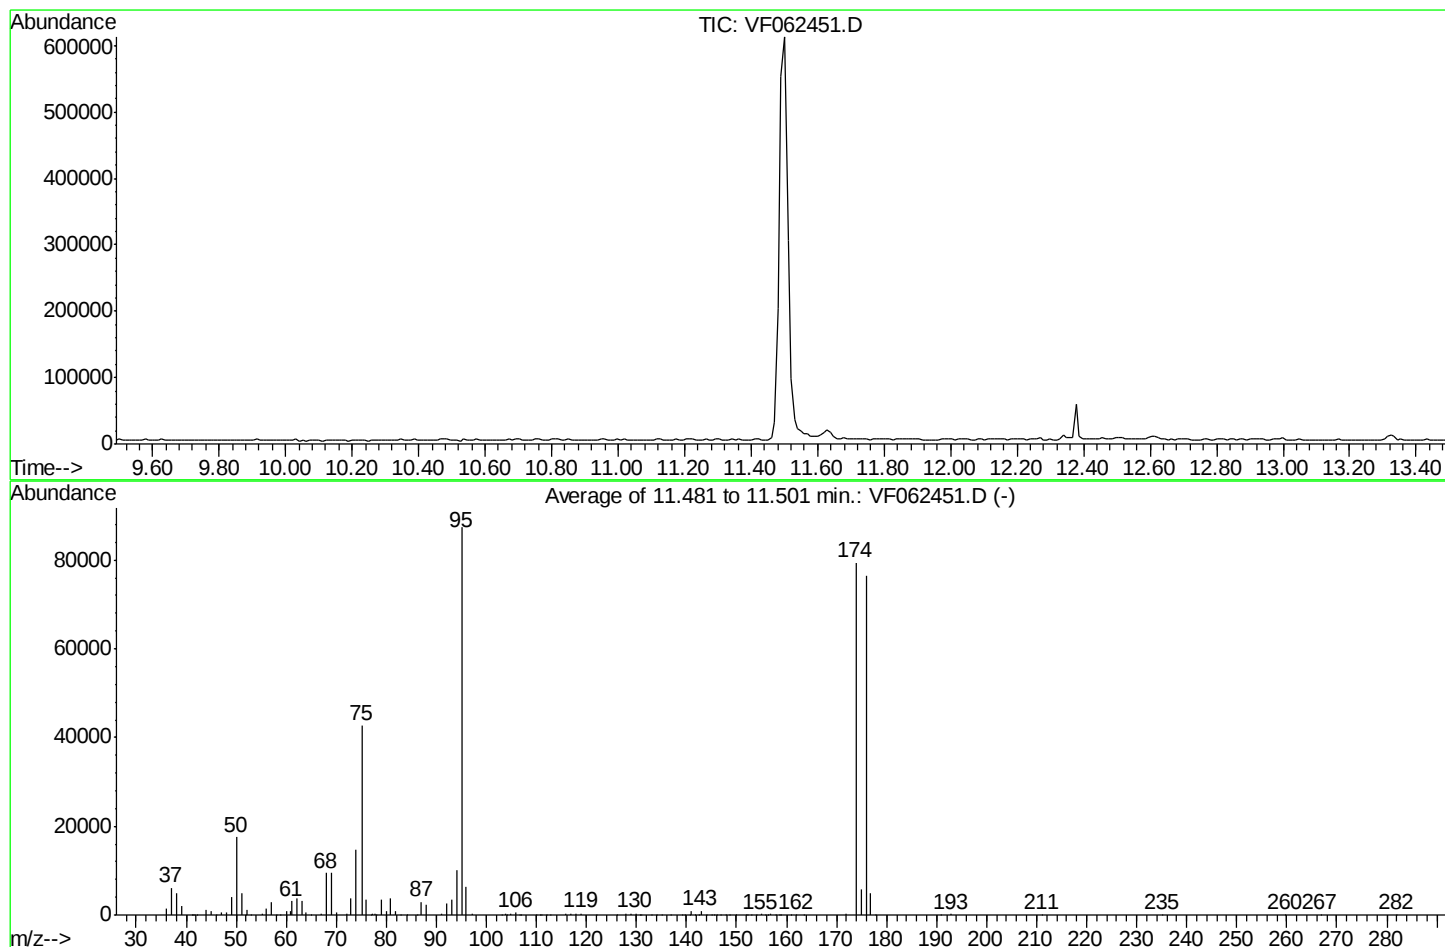

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1104

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	17544	PASS
75	95	30	60	48.9	42701	PASS
95	95	100	100	100.0	87389	PASS
96	95	5	9	7.3	6380	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.9	79429	PASS
175	174	5	9	7.4	5901	PASS
176	174	95	101	96.2	76408	PASS
177	176	5	9	6.6	5012	PASS