


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF051119\
 Data File : VF062473.D
 Acq On : 11 May 2019 21:47
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_F/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Title : SW846 8260
 Last Update : Tue May 07 04:34:57 2019

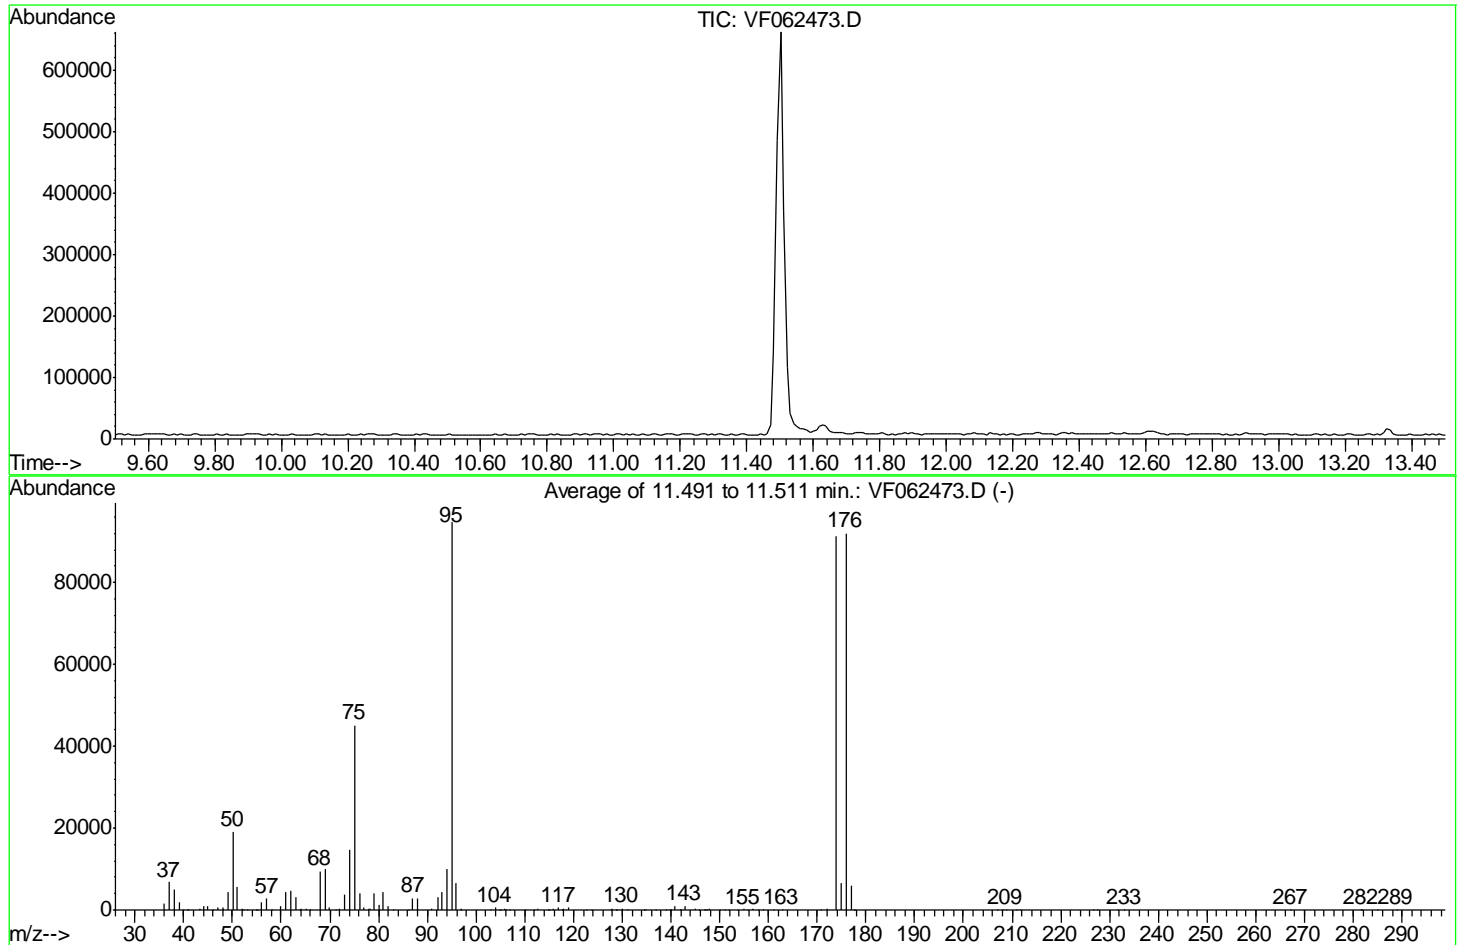

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	19075	PASS
75	95	30	60	47.5	45018	PASS
95	95	100	100	100.0	94677	PASS
96	95	5	9	6.9	6541	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	96.4	91293	PASS
175	174	5	9	7.2	6529	PASS
176	174	95	101	100.8	91981	PASS
177	176	5	9	6.4	5922	PASS