

Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF051219\
 Data File : VF062509.D
 Acq On : 12 May 2019 18:05
 Operator : FY/SY
 Sample : K2719-16RE
 Misc : 6.44g/5mL/MSVOA F/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 P026-SS010-1218-01RE

Quant Time: May 15 02:04:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 07 04:34:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.08	168	162984	50.00	ug/l	0.03
34) 1,4-Difluorobenzene	5.80	114	205547	50.00	ug/l	0.03
63) Chlorobenzene-d5	9.93	117	137369	50.00	ug/l	0.03
72) 1,4-Dichlorobenzene-d4	12.62	152	53781	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.05	65	58893	38.24	ug/l	0.03
Spiked Amount	50.000		Recovery	=	76.48%	
35) Dibromofluoromethane	4.33	113	74412	45.44	ug/l	0.03
Spiked Amount	50.000		Recovery	=	90.88%	
50) Toluene-d8	7.73	98	136322	34.39	ug/l	0.03
Spiked Amount	50.000		Recovery	=	68.78%	
62) 4-Bromofluorobenzene	11.51	95	44122	24.67	ug/l	0.02
Spiked Amount	50.000		Recovery	=	49.34%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF051219\
Data File : VF062509.D
Acq On : 12 May 2019 18:05
Operator : FY/SY
Sample : K2719-16RE
Misc : 6.44g/5mL/MSVOA F/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
P026-SS010-1218-01RE

Quant Time: May 15 02:04:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Quant Title : SW846 8260
QLast Update : Tue May 07 04:34:57 2019
Response via : Initial Calibration

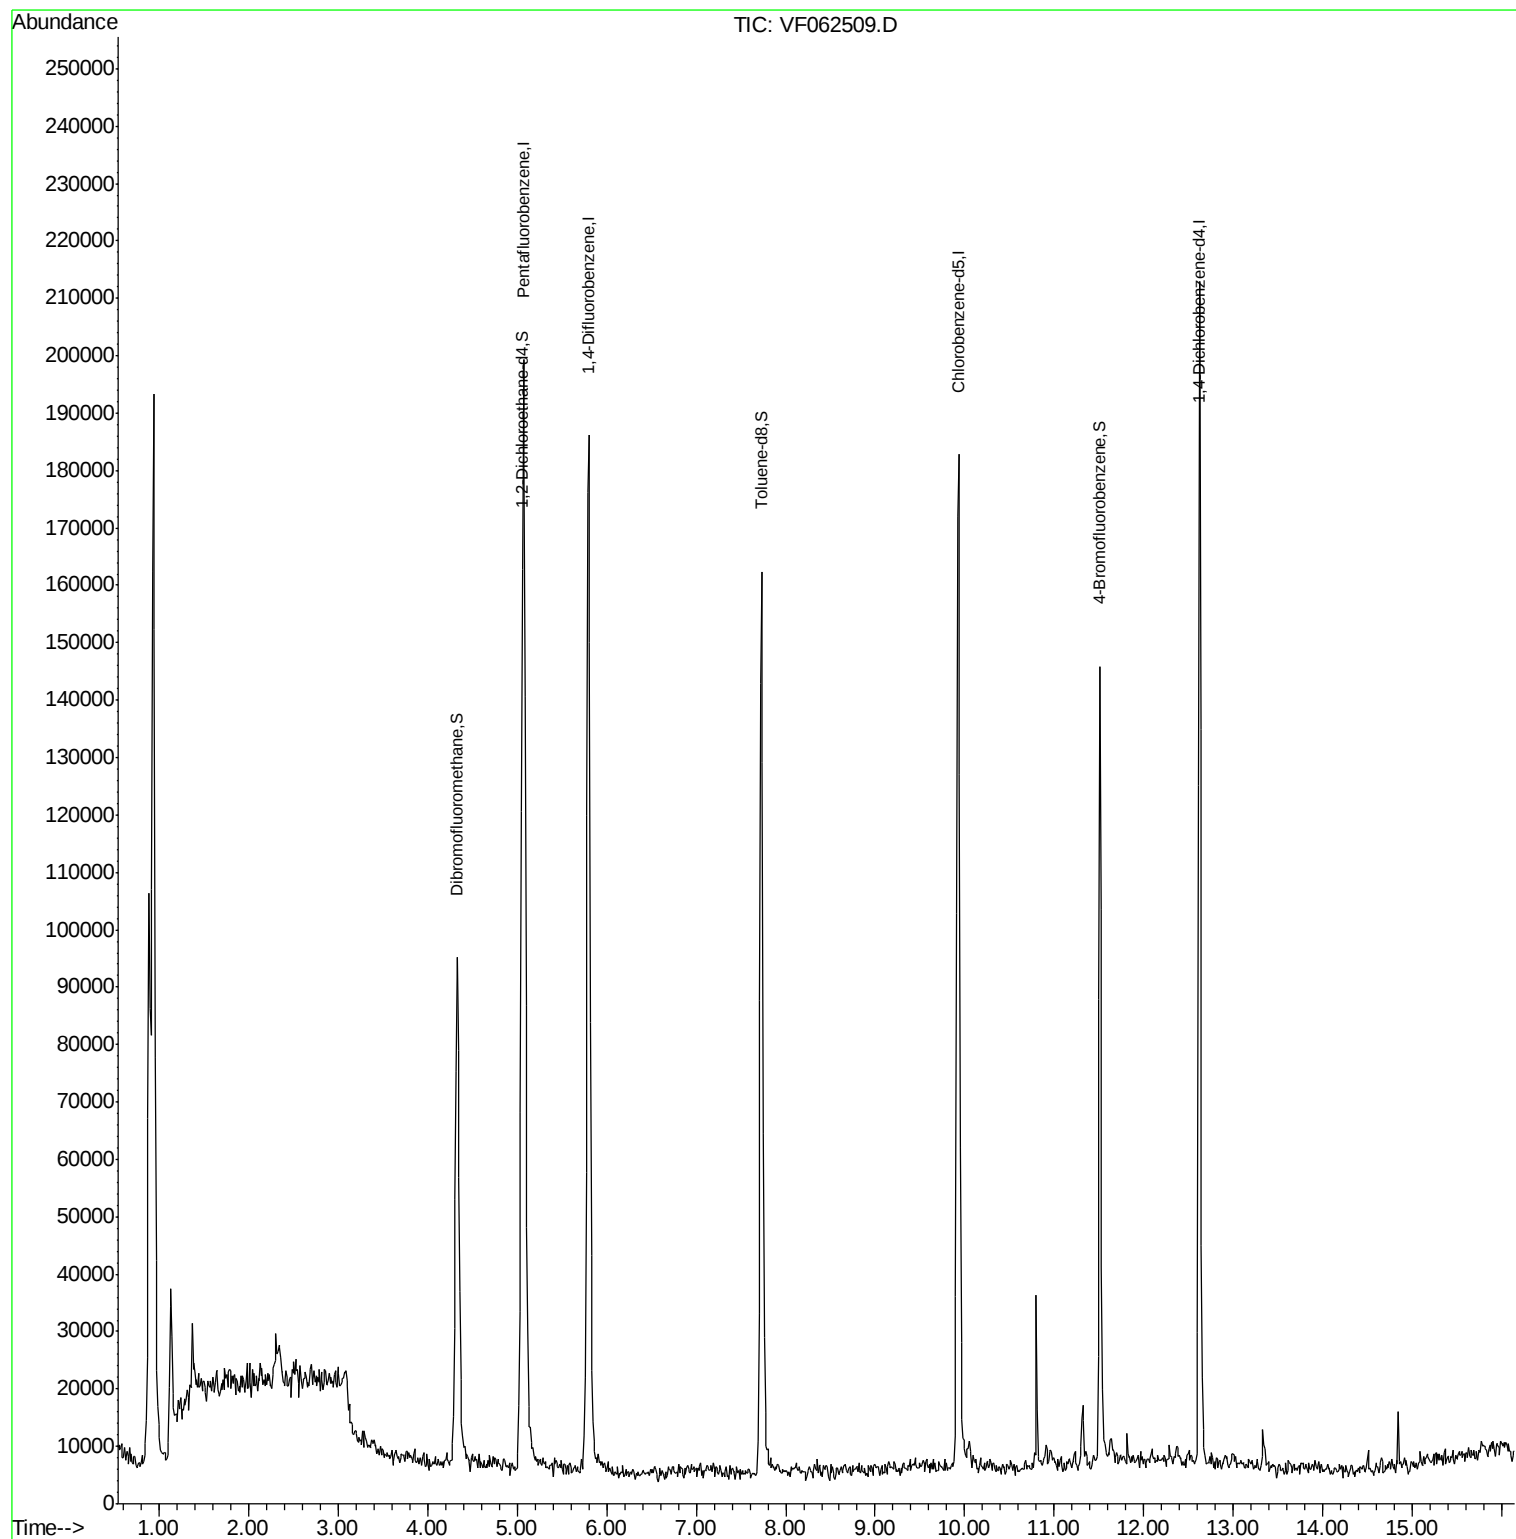



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.08 min Scan# 461

Delta R.T. 0.03 min

Lab File: VF062509.D

Acq: 12 May 2019 18:05

Instrument :

MSVOA_F

ClientSampleId :


P026-SS010-1218-01RE

Tot Ion:168 Resp: 162984

Ion Ratio Lower Upper




168 100

99 54.8 45.9 68.9

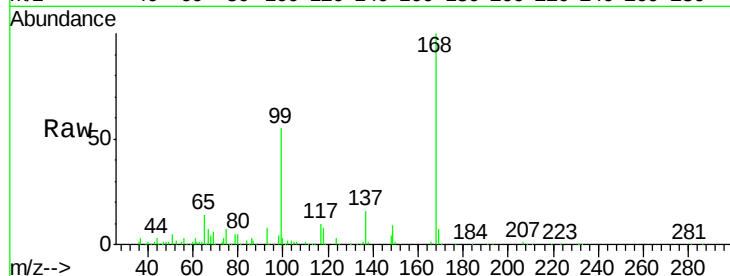

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VF0

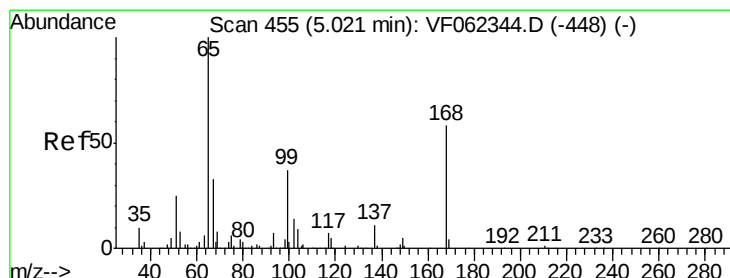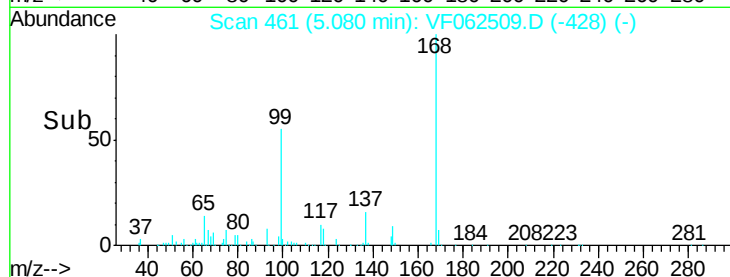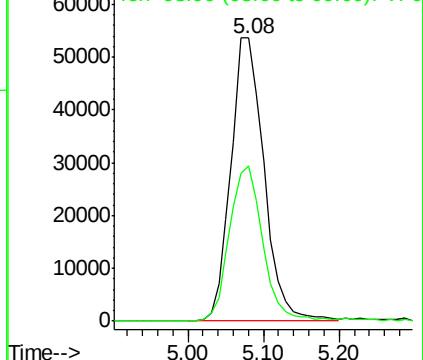

#33

1,2-Dichloroethane-d4

Concen: 38.236 ug/l

RT: 5.05 min Scan# 458

Delta R.T. 0.03 min

Lab File: VF062509.D


Acq: 12 May 2019 18:05

Tgt Ion: 65 Resp: 58893

Ion Ratio Lower Upper



65 100


67 44.0 0.0 85.8

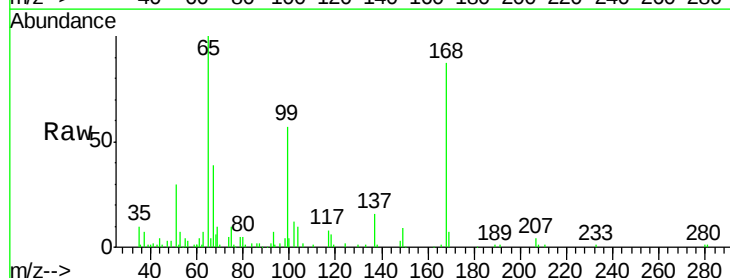

Abundance Ion 64.90 (64.60 to 65.60): VF0

Ion 66.90 (66.60 to 67.60): VF0

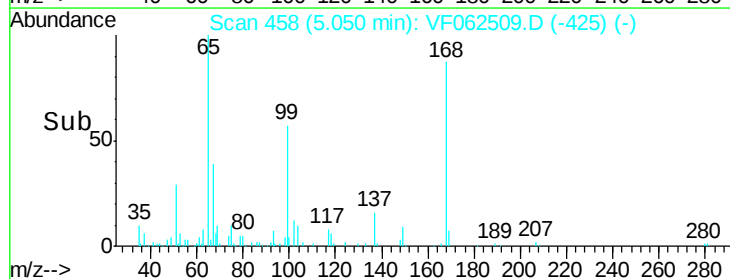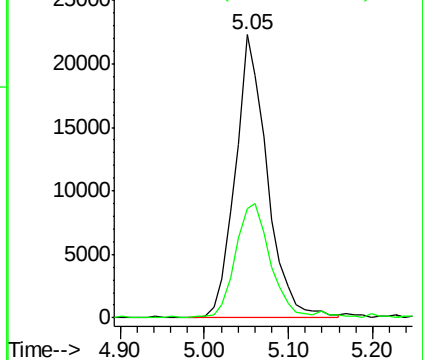

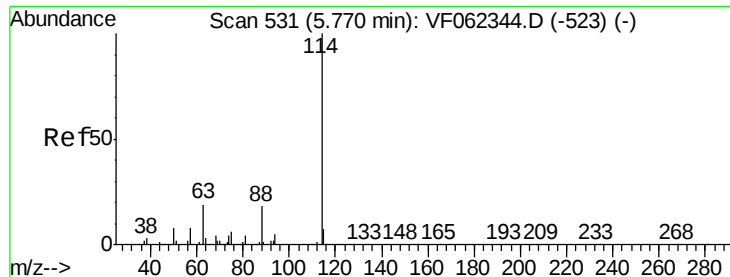

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.80 min Scan# 534

Delta R.T. 0.03 min

Lab File: VF062509.D

Acq: 12 May 2019 18:05

Instrument :

MSVOA_F

ClientSampleId :

P026-SS010-1218-01RE


Tot Ion:114 Resp: 205547

Ion Ratio Lower Upper

114 100

63 20.5 0.0 37.4




88 20.0 0.0 36.4

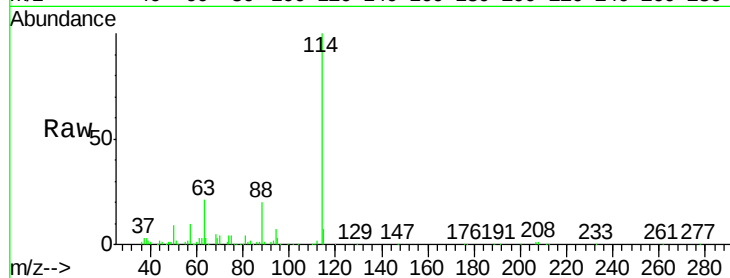

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 87.90 (87.60 to 88.60): VF0

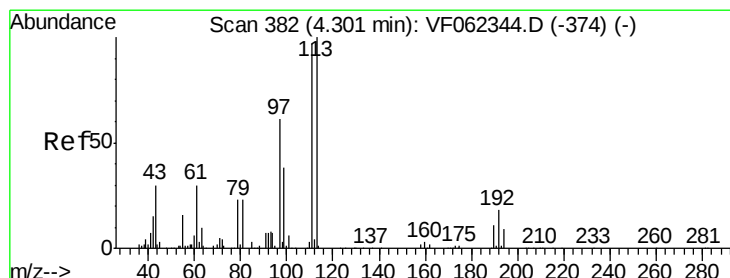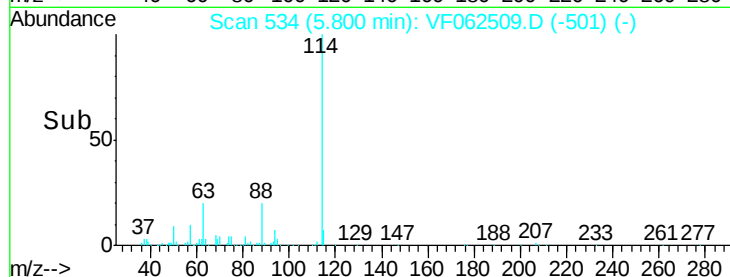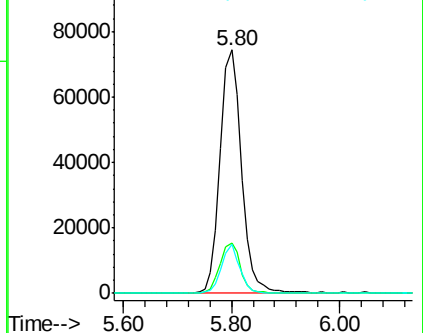

#35

Dibromofluoromethane

Concen: 45.441 ug/l

RT: 4.33 min Scan# 385

Delta R.T. 0.03 min

Lab File: VF062509.D

Acq: 12 May 2019 18:05


Tgt Ion:113 Resp: 74412

Ion Ratio Lower Upper

113 100

111 100.4 79.4 119.0



192 20.2 16.0 24.0

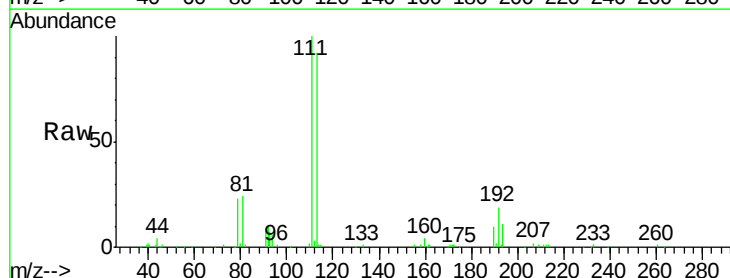


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

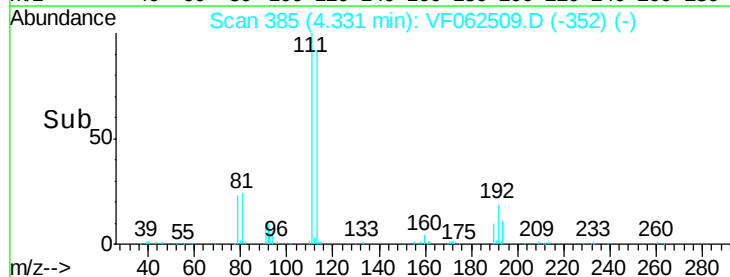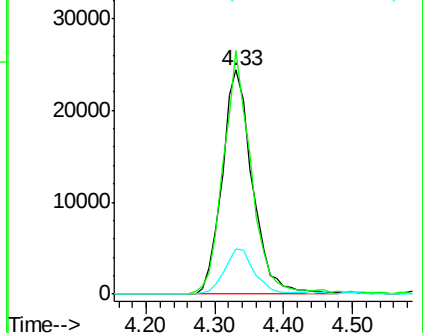

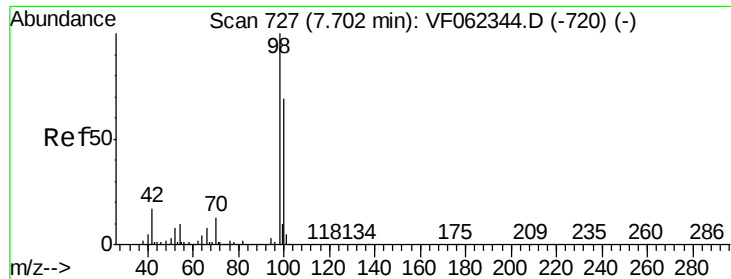

#50

Toluene-d8

Concen: 34.390 ug/l

RT: 7.73 min Scan# 730

Delta R.T. 0.03 min

Lab File: VF062509.D

Acq: 12 May 2019 18:05

Instrument :

MSVOA_F

ClientSampleId :


P026-SS010-1218-01RE

Tot Ion: 98 Resp: 136322

Ion Ratio Lower Upper

98 100

100 67.2 53.3 79.9

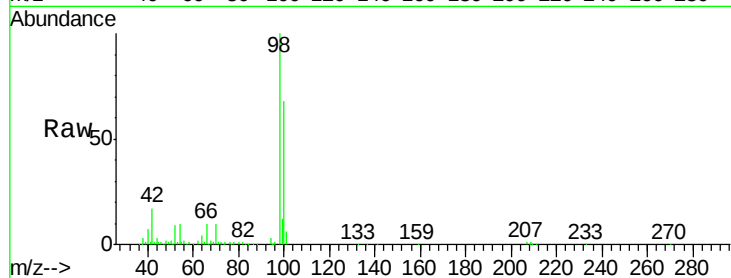

Abundance Ion 98.00 (97.70 to 98.70): VF0

Ion 100.00 (99.70 to 100.70): VF0

60000

50000

40000

30000



20000

10000

0

7.60 7.70 7.80 7.90

Time-->

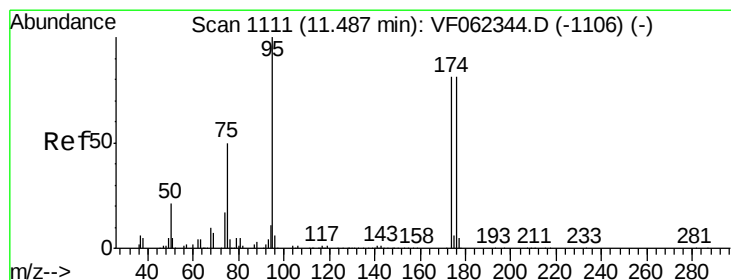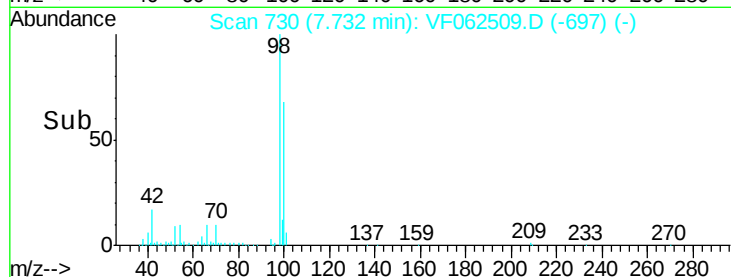

#62

4-Bromofluorobenzene

Concen: 24.671 ug/l

RT: 11.51 min Scan# 1113

Delta R.T. 0.02 min

Lab File: VF062509.D

Acq: 12 May 2019 18:05


Tgt Ion: 95 Resp: 44122

Ion Ratio Lower Upper

95 100

174 100.4 0.0 191.8

176 98.2 0.0 193.2

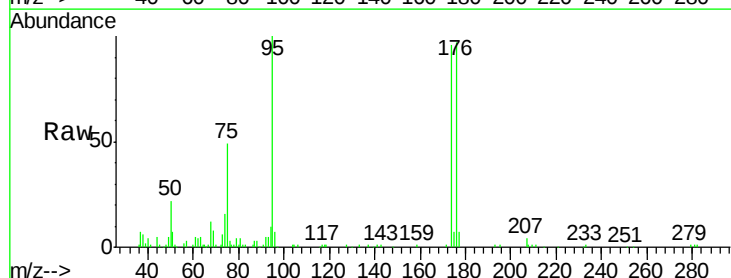

Abundance Ion 94.90 (94.60 to 95.60): VF0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

30000


20000


10000

0

11.40 11.50 11.60

Time-->

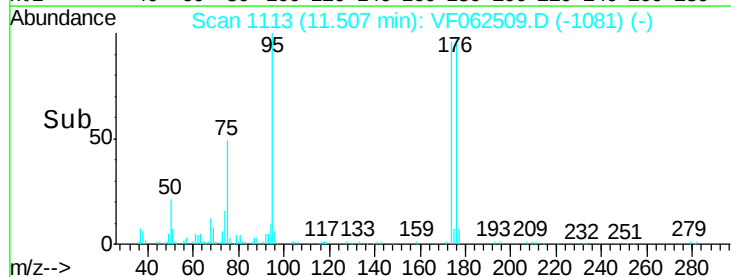

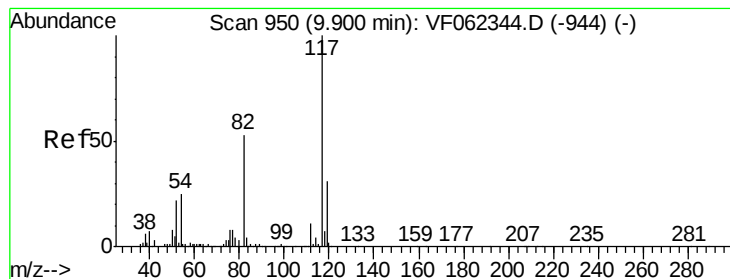

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.93 min Scan# 953

Delta R.T. 0.03 min

Lab File: VF062509.D

Acq: 12 May 2019 18:05

Instrument :

MSVOA_F

ClientSampleId :

P026-SS010-1218-01RE


Tot Ion:117 Resp: 137369

Ion Ratio Lower Upper

117 100

82 51.3 42.2 63.2




119 29.9 25.0 37.4

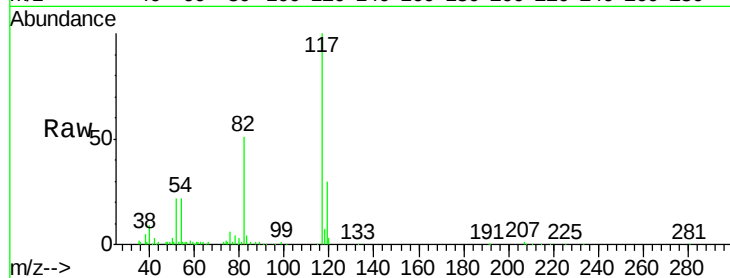

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

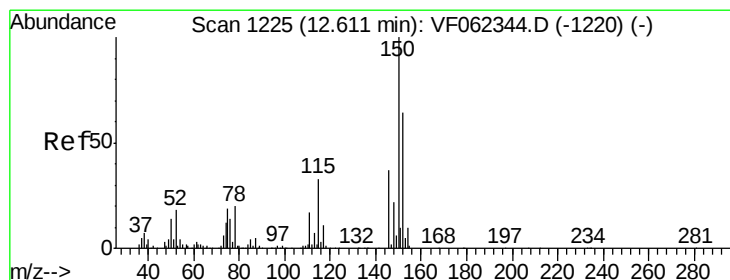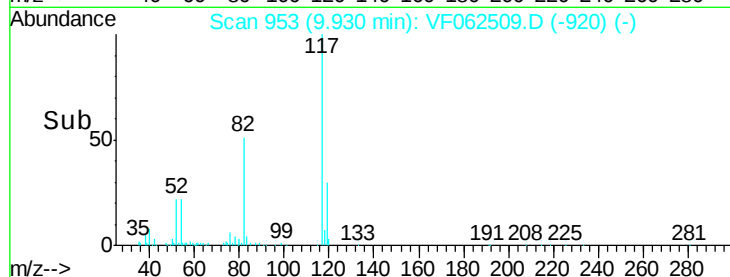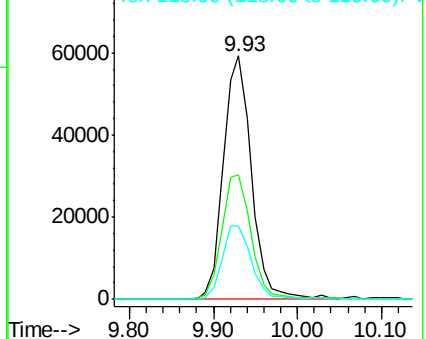

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.62 min Scan# 1226

Delta R.T. 0.01 min

Lab File: VF062509.D

Acq: 12 May 2019 18:05


Tgt Ion:152 Resp: 53781

Ion Ratio Lower Upper

152 100

115 55.3 26.4 79.2

150 156.1 0.0 335.0

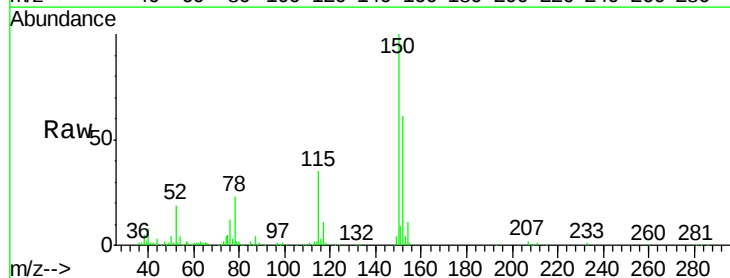

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

