

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF051219\
 Data File : VF062534.D
 Acq On : 13 May 2019 7:07
 Operator : FY/SY
 Sample : K2734-15RE
 Misc : 5.20g/5mL/MSVOA F/SOIL
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 P026-SS013-1824-01RE

Quant Time: May 13 08:03:38 2019
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 07 04:34:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.08	168	74348	50.00	ug/l	0.03
34) 1,4-Difluorobenzene	5.79	114	89131	50.00	ug/l	0.02
63) Chlorobenzene-d5	9.93	117	72457	50.00	ug/l	0.03
72) 1,4-Dichlorobenzene-d4	12.62	152	32746	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.05	65	26494	37.71	ug/l	0.03
Spiked Amount	50.000		Recovery	=	75.42%	
35) Dibromofluoromethane	4.33	113	34166	48.11	ug/l	0.03
Spiked Amount	50.000		Recovery	=	96.22%	
50) Toluene-d8	7.73	98	67396	39.21	ug/l	0.03
Spiked Amount	50.000		Recovery	=	78.42%	
62) 4-Bromofluorobenzene	11.51	95	25091	32.35	ug/l	0.02
Spiked Amount	50.000		Recovery	=	64.70%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF051219\
Data File : VF062534.D
Acq On : 13 May 2019 7:07
Operator : FY/SY
Sample : K2734-15RE
Misc : 5.20g/5mL/MSVOA F/SOIL
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
P026-SS013-1824-01RE

Quant Time: May 13 08:03:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
Quant Title : SW846 8260
QLast Update : Tue May 07 04:34:57 2019
Response via : Initial Calibration

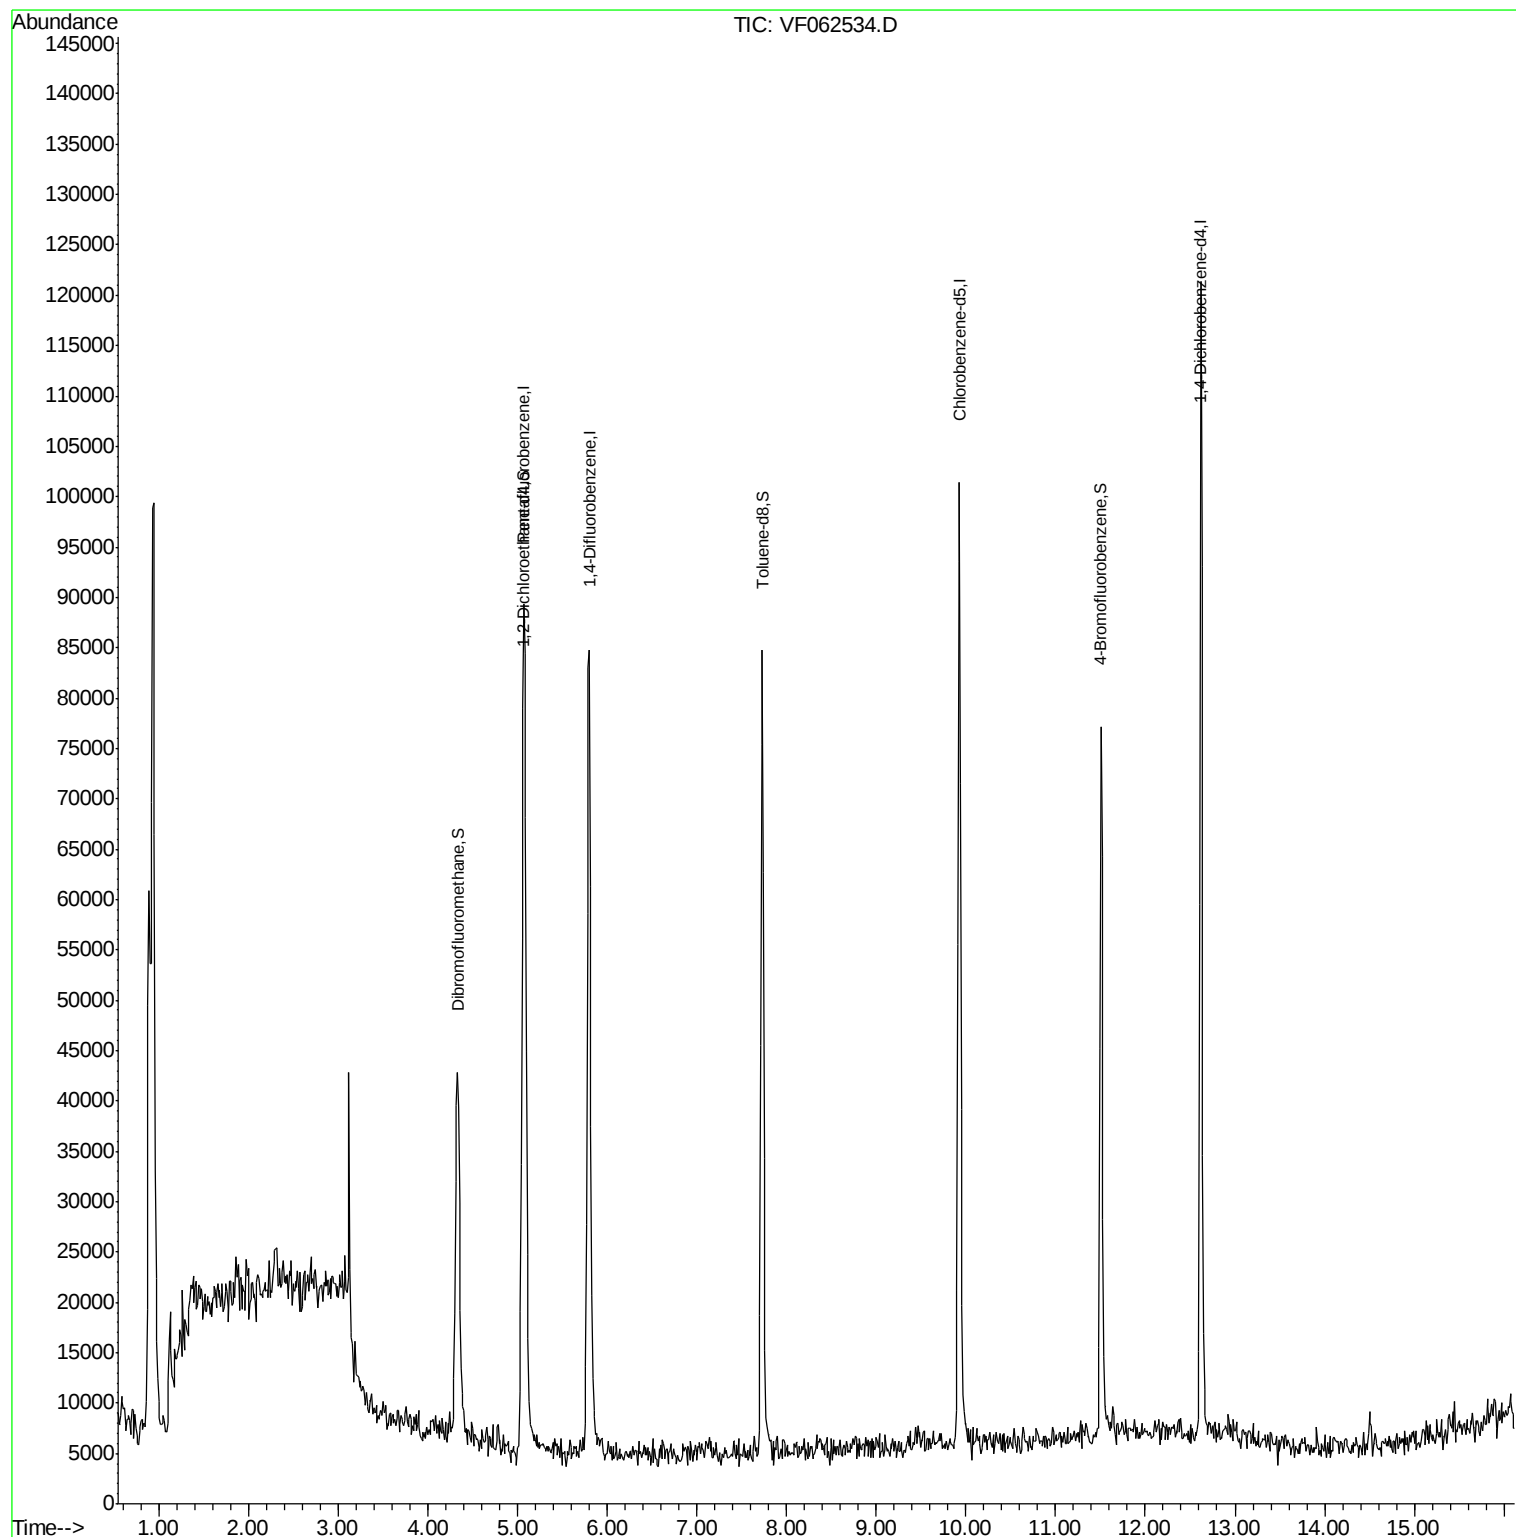

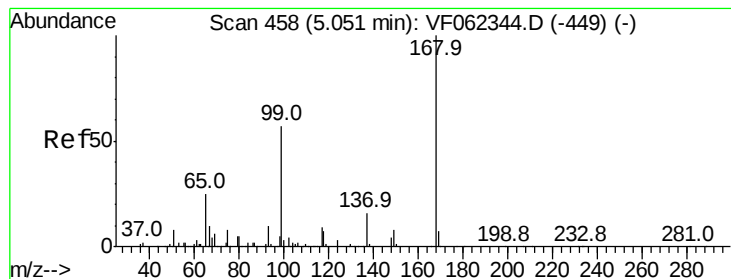

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.08 min Scan# 461

Delta R.T. 0.03 min

Lab File: VF062534.D

Acq: 13 May 2019 7:07

Instrument :

MSVOA_F

ClientSampleId :


P026-SS013-1824-01RE

Tot Ion:168 Resp: 74348




Ion Ratio Lower Upper

168 100

99 52.8 45.9 68.9

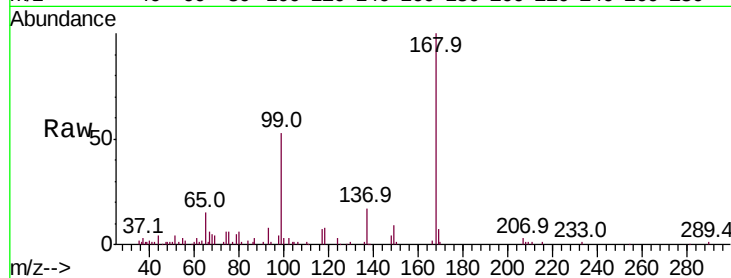

Abundance Ion 167.90 (167.60 to 168.60): VF0

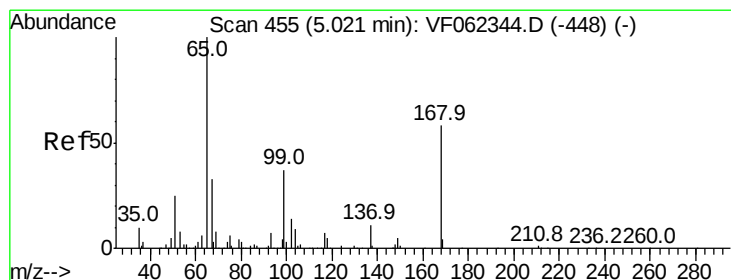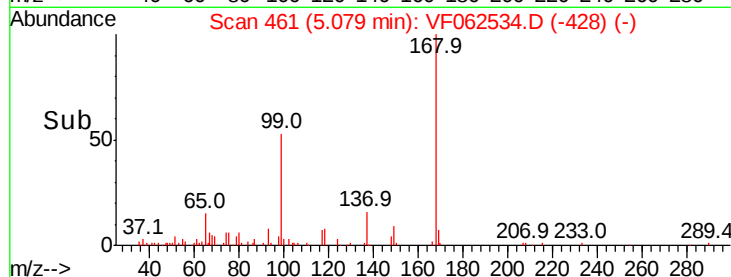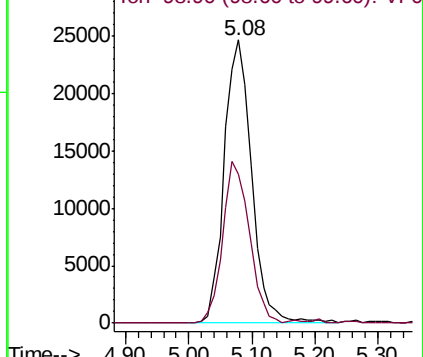

#33

1,2-Dichloroethane-d4

Concen: 37.707 ug/l

RT: 5.05 min Scan# 458

Delta R.T. 0.03 min

Lab File: VF062534.D


Acq: 13 May 2019 7:07

Tgt Ion: 65 Resp: 26494



Ion Ratio Lower Upper


65 100

67 48.2 0.0 85.8

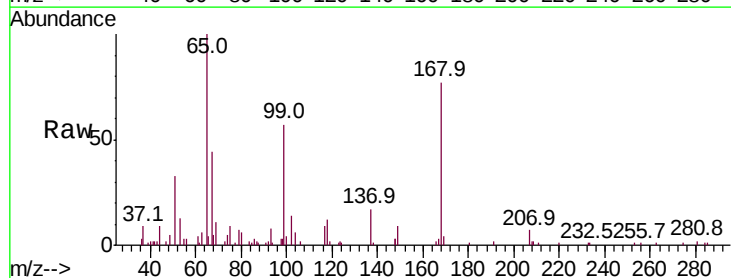

Abundance Ion 64.90 (64.60 to 65.60): VF0

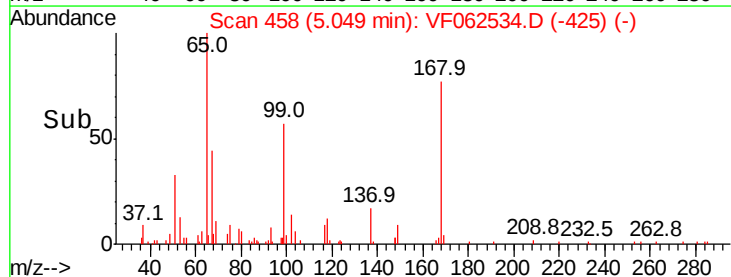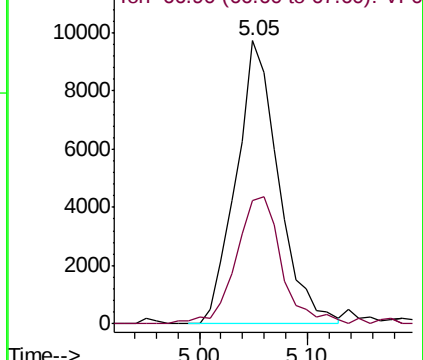

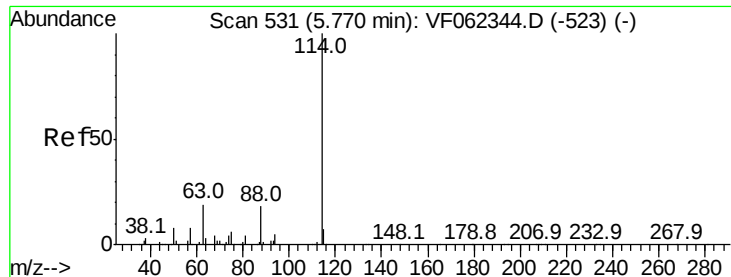

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.79 min Scan# 533

Delta R.T. 0.02 min

Lab File: VF062534.D

Acq: 13 May 2019 7:07

Instrument :

MSVOA_F

ClientSampleId :

P026-SS013-1824-01RE


Tot Ion:114 Resp: 89131

Ion Ratio Lower Upper

114 100

63 18.9 0.0 37.4




88 17.0 0.0 36.4

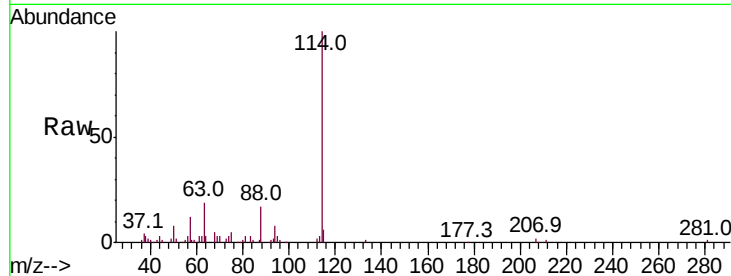

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 87.90 (87.60 to 88.60): VF0

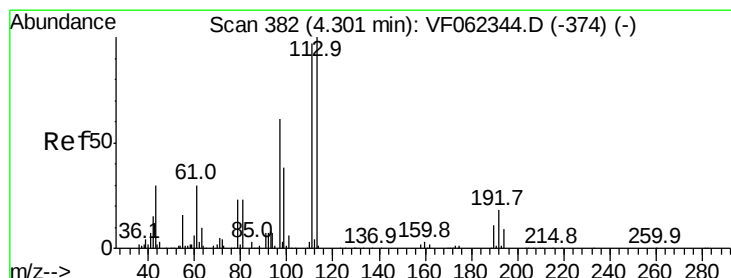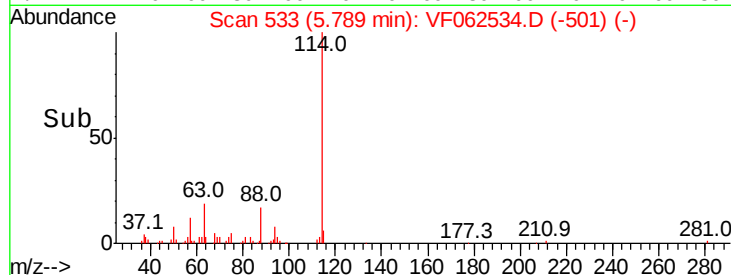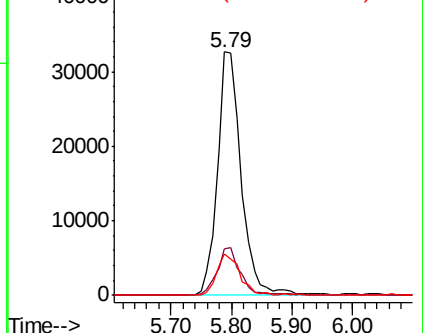

#35

Dibromofluoromethane

Concen: 48.115 ug/l

RT: 4.33 min Scan# 385

Delta R.T. 0.03 min

Lab File: VF062534.D

Acq: 13 May 2019 7:07


Tgt Ion:113 Resp: 34166

Ion Ratio Lower Upper

113 100

111 98.3 79.4 119.0



192 19.7 16.0 24.0

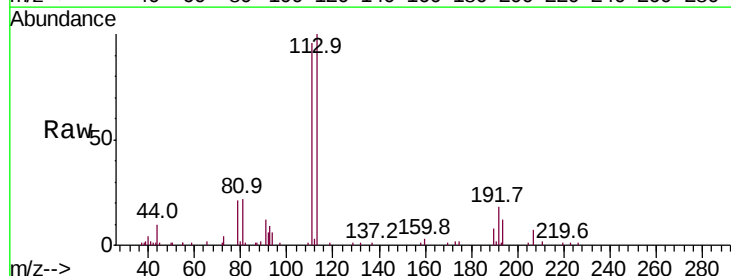


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

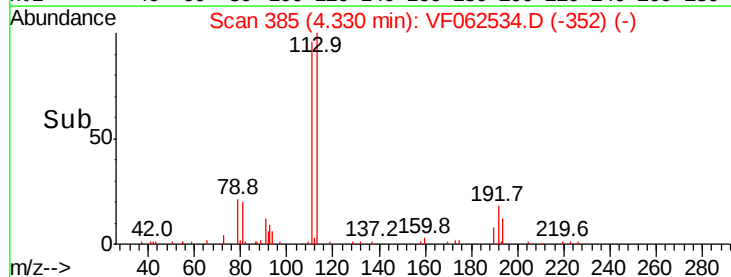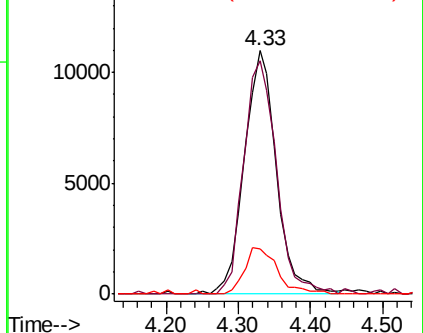

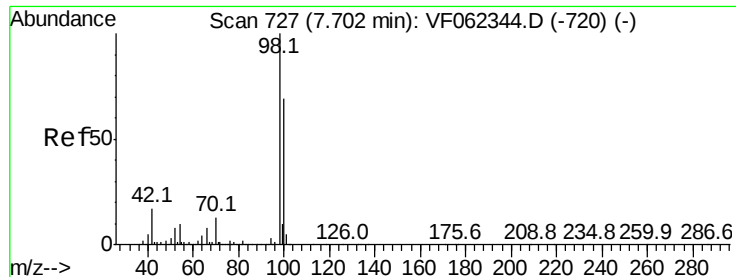

#50

Toluene-d8

Concen: 39.209 ug/l

RT: 7.73 min Scan# 730

Delta R.T. 0.03 min

Lab File: VF062534.D

Acq: 13 May 2019 7:07

Instrument :

MSVOA_F

ClientSampleId :


P026-SS013-1824-01RE

Tot Ion: 98 Resp: 67396

Ion Ratio Lower Upper

98 100

100 65.9 53.3 79.9

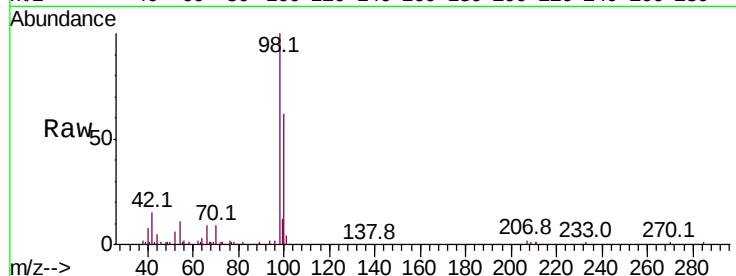

Abundance Ion 98.00 (97.70 to 98.70): VF0

Ion 100.00 (99.70 to 100.70): VF

30000



20000

10000

0

7.60 7.70 7.80 7.90

Time-->

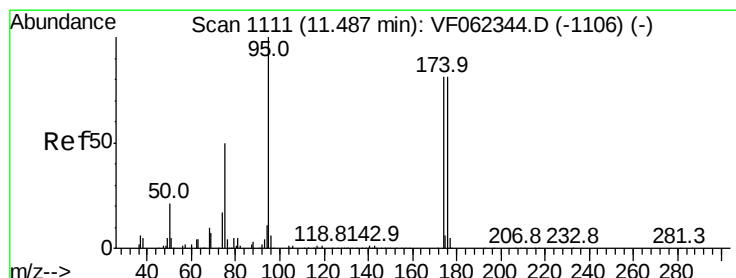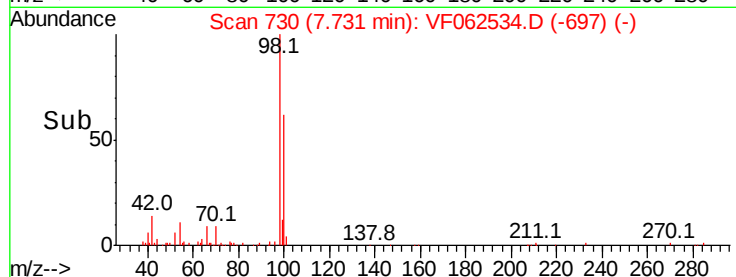

#62

4-Bromofluorobenzene

Concen: 32.355 ug/l

RT: 11.51 min Scan# 1113

Delta R.T. 0.02 min

Lab File: VF062534.D

Acq: 13 May 2019 7:07


Tgt Ion: 95 Resp: 25091

Ion Ratio Lower Upper

95 100

174 91.0 0.0 191.8

176 91.1 0.0 193.2

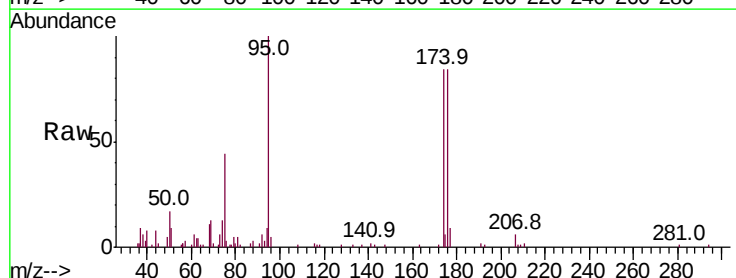

Abundance Ion 94.90 (94.60 to 95.60): VF0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

15000


10000


5000

0

11.40 11.50 11.60

Time-->




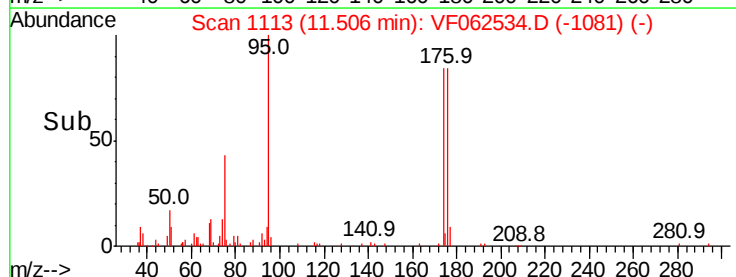


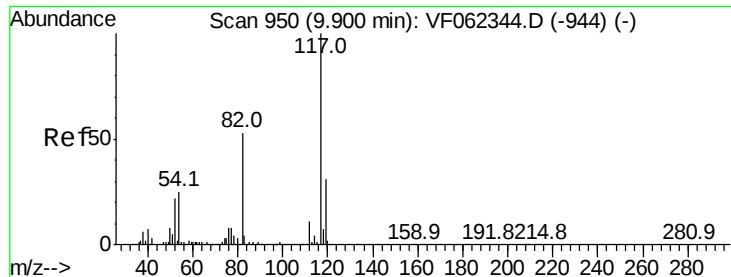

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.93 min Scan# 953
Delta R.T. 0.03 min
Lab File: VF062534.D
Acq: 13 May 2019 7:07

Instrument :
MSVOA_F
ClientSampleId :
P026-SS013-1824-01RE

Tot Ion	Ratio	Lower	Upper
117	100		
82	53.4	42.2	63.2
119	34.3	25.0	37.4

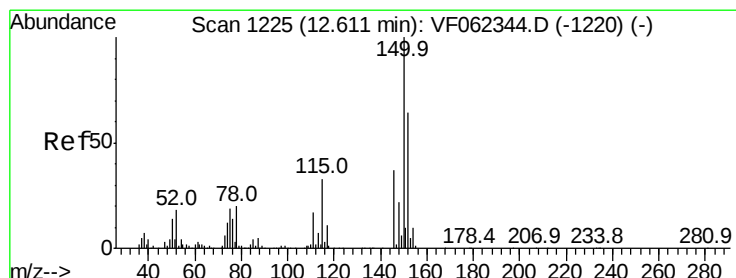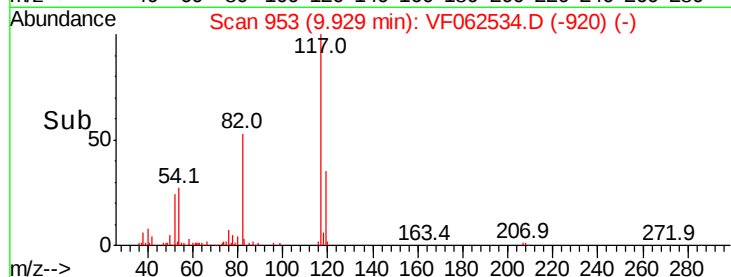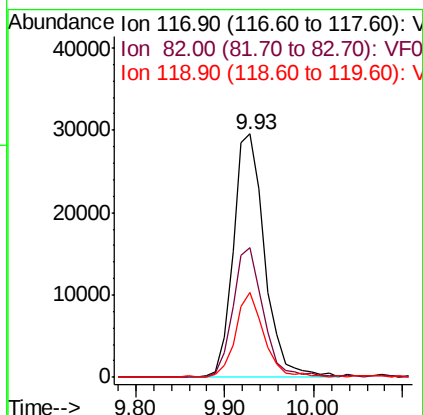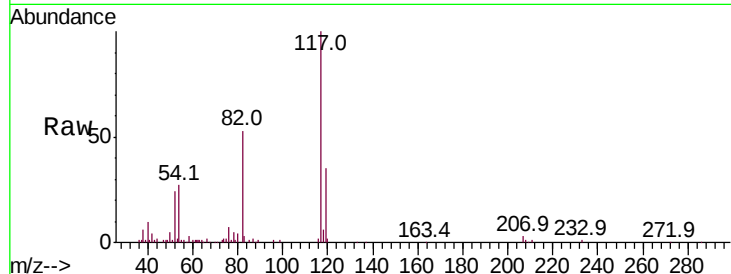

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.62 min Scan# 1226
Delta R.T. 0.01 min
Lab File: VF062534.D
Acq: 13 May 2019 7:07

Tgt Ion	Ratio	Lower	Upper
152	100		
115	48.9	26.4	79.2
150	146.0	0.0	335.0

