


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF051219\
 Data File : VF062515.D
 Acq On : 12 May 2019 20:52
 Operator : FY/SY
 Sample : BFB
 Misc : 5.85µ/5mL/MSVOA F/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Title : SW846 8260
 Last Update : Tue May 07 04:34:57 2019

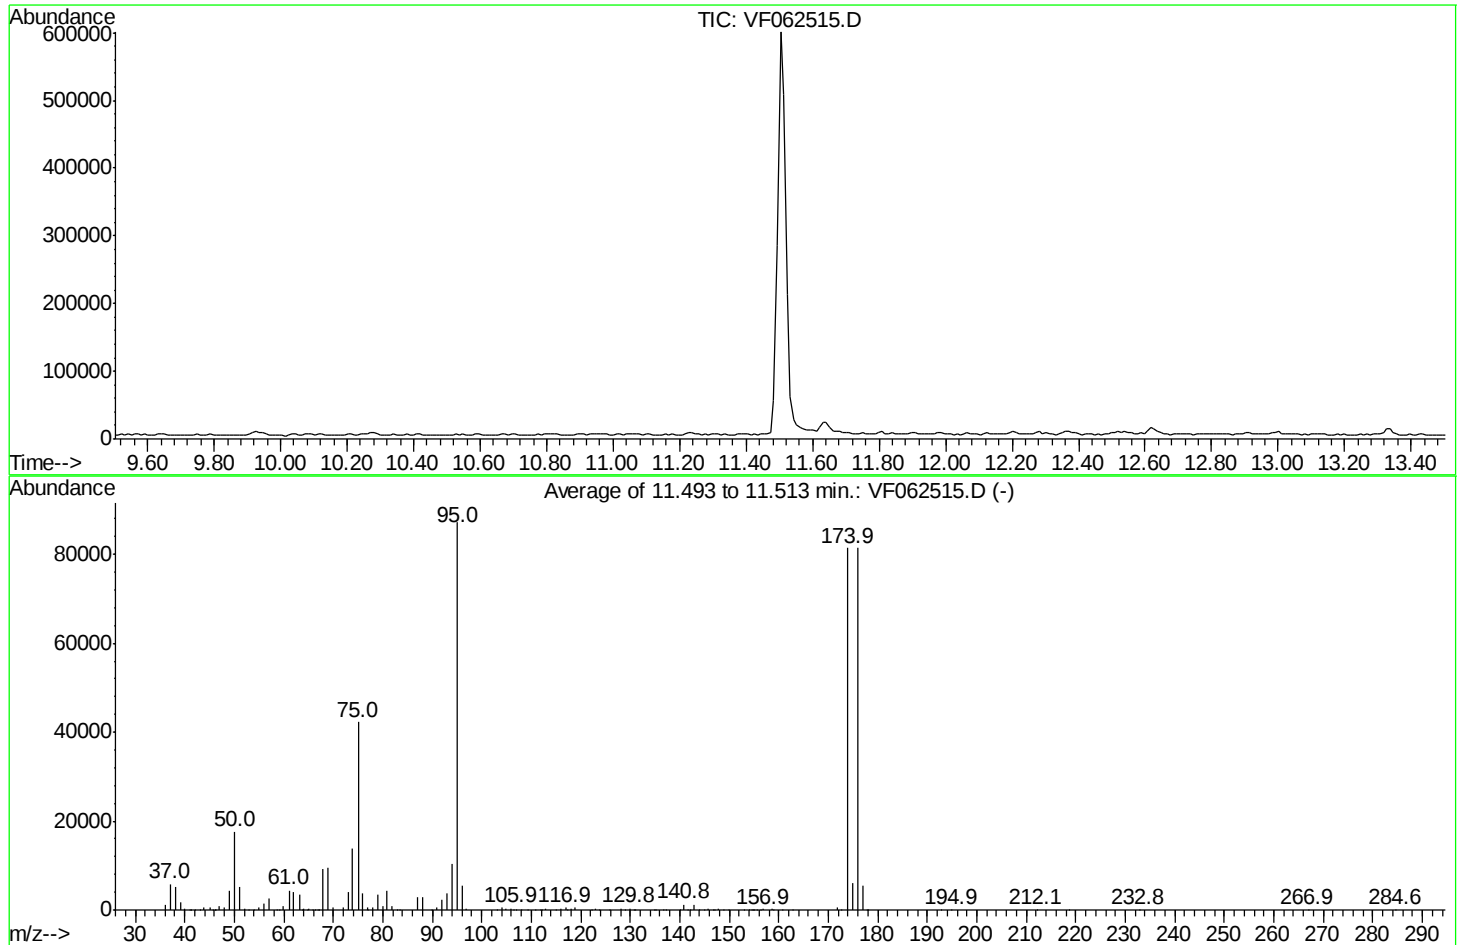

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	17707	PASS
75	95	30	60	48.5	42304	PASS
95	95	100	100	100.0	87226	PASS
96	95	5	9	6.4	5604	PASS
173	174	0.00	2	0.1	83	PASS
174	95	50	100	93.4	81501	PASS
175	174	5	9	7.6	6154	PASS
176	174	95	101	99.9	81397	PASS
177	176	5	9	6.7	5449	PASS