


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF051319\
 Data File : VF062538.D
 Acq On : 13 May 2019 12:16
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Title : SW846 8260
 Last Update : Tue May 07 04:34:57 2019

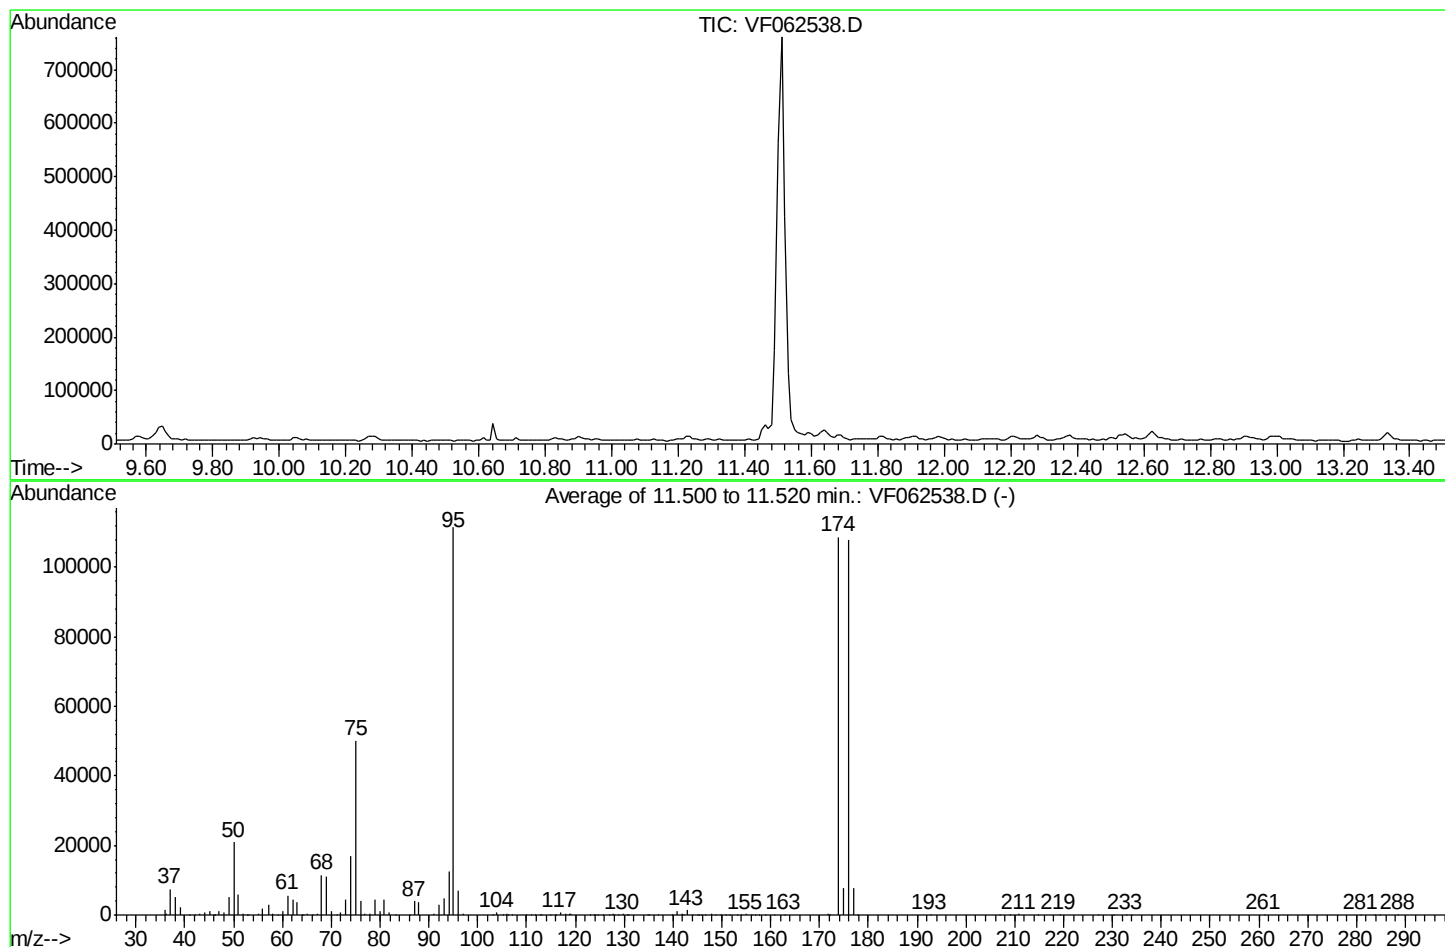

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	20924	PASS
75	95	30	60	44.9	50045	PASS
95	95	100	100	100.0	111434	PASS
96	95	5	9	6.4	7167	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	97.5	108672	PASS
175	174	5	9	7.2	7796	PASS
176	174	95	101	99.1	107701	PASS
177	176	5	9	7.0	7573	PASS