


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF051319\
 Data File : VF062560.D
 Acq On : 14 May 2019 00:19
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82F050619S.M
 Title : SW846 8260
 Last Update : Tue May 07 04:34:57 2019

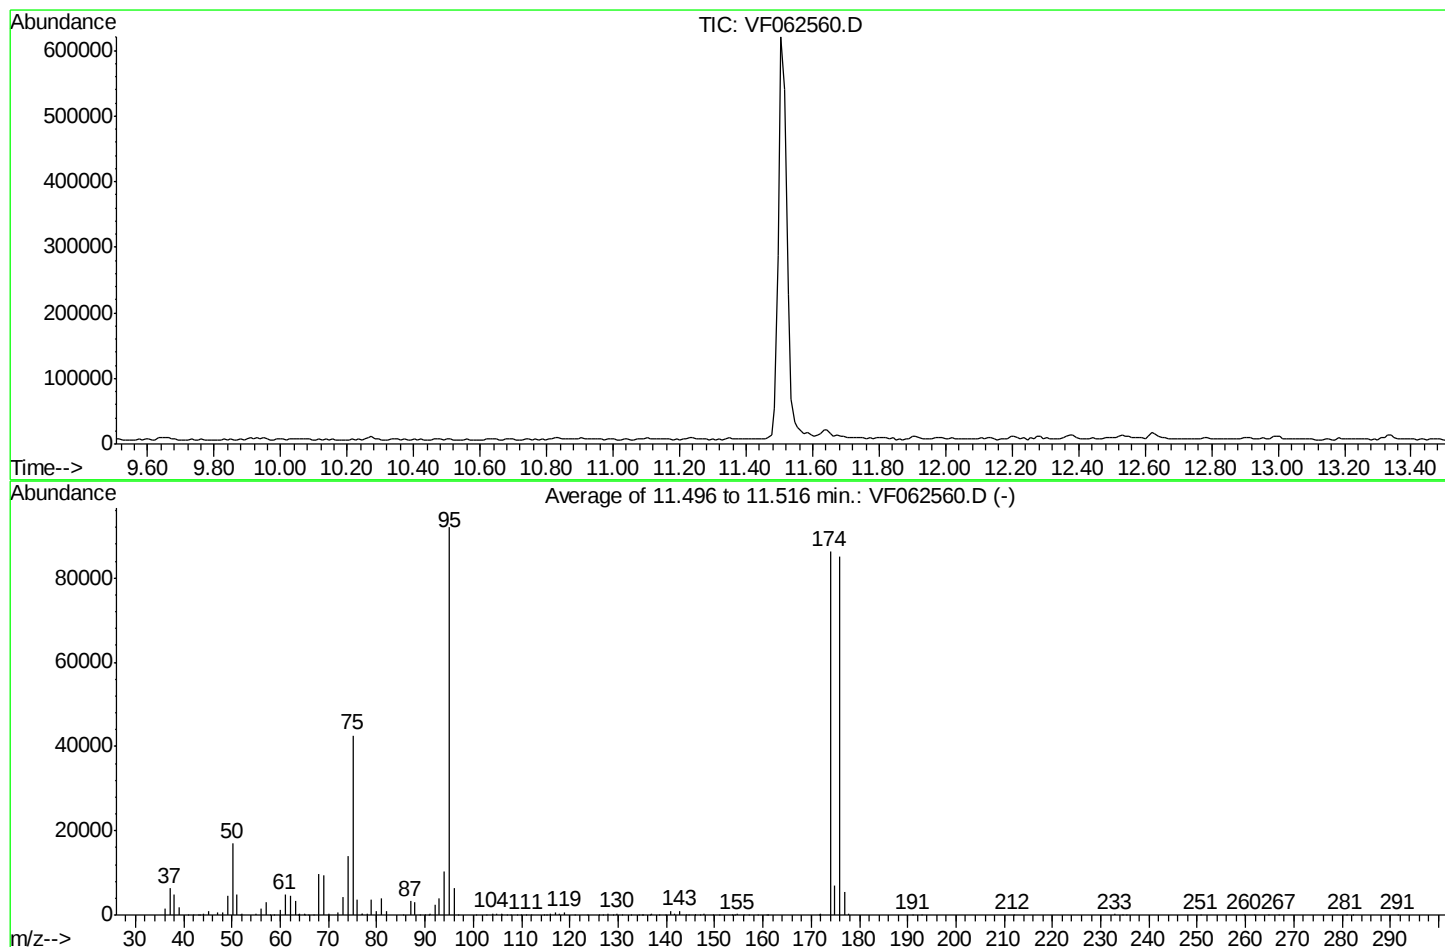

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	16949	PASS
75	95	30	60	46.4	42666	PASS
95	95	100	100	100.0	92008	PASS
96	95	5	9	7.1	6521	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.7	86194	PASS
175	174	5	9	8.0	6918	PASS
176	174	95	101	98.7	85066	PASS
177	176	5	9	6.5	5549	PASS