


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF051419\
 Data File : VF062582.D
 Acq On : 14 May 2019 14:22
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F051419S.M
 Title : SW846 8260
 Last Update : Wed May 15 05:06:28 2019

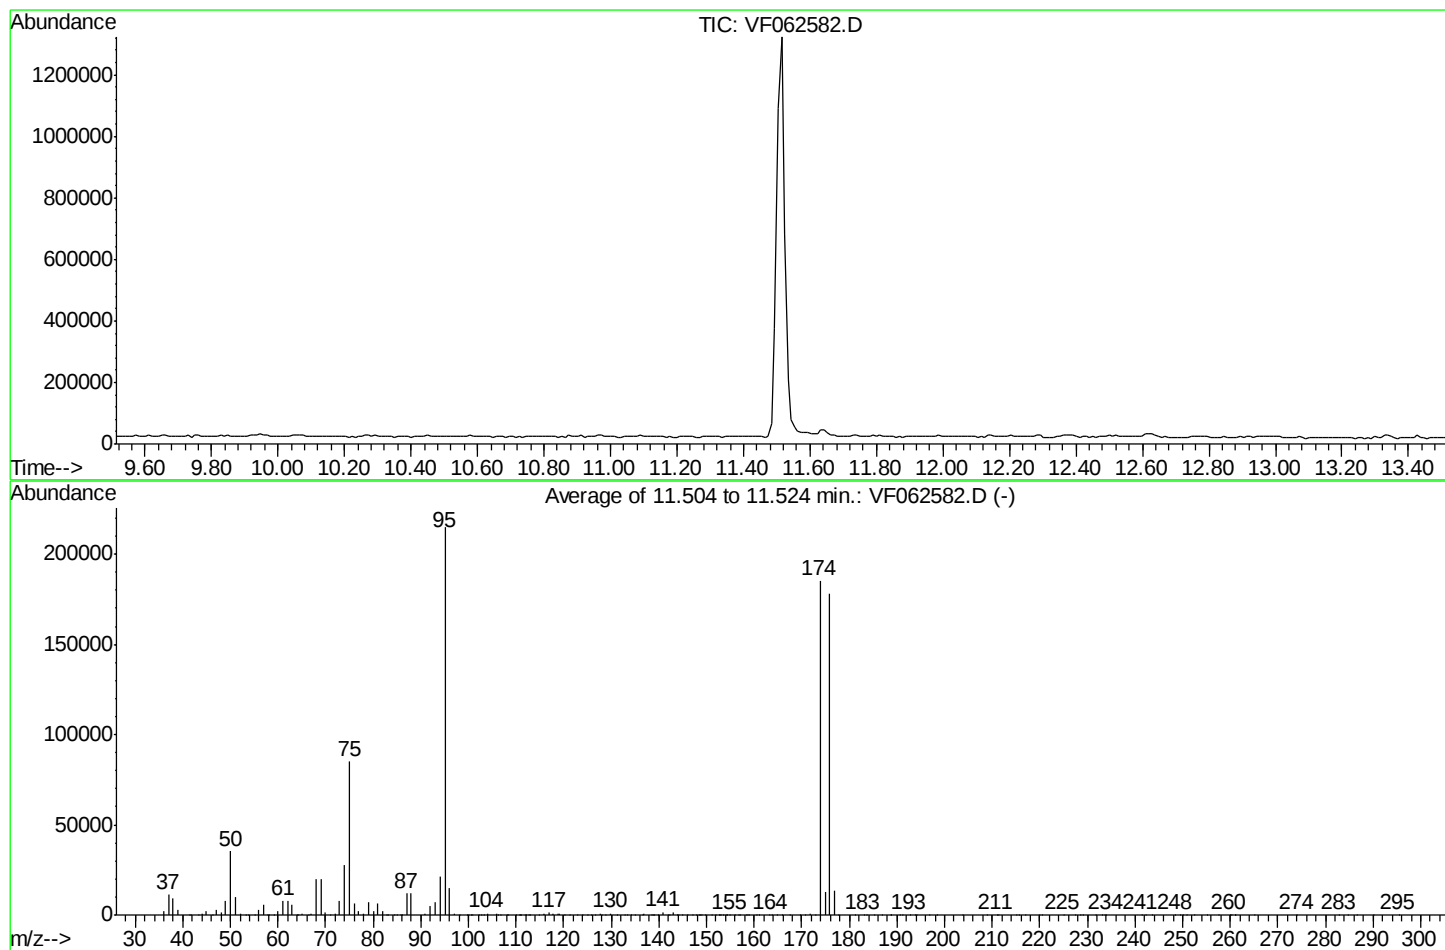

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	35279	PASS
75	95	30	60	39.5	84900	PASS
95	95	100	100	100.0	214885	PASS
96	95	5	9	7.0	14987	PASS
173	174	0.00	2	0.1	156	PASS
174	95	50	100	86.3	185429	PASS
175	174	5	9	6.9	12788	PASS
176	174	95	101	96.0	178026	PASS
177	176	5	9	7.5	13280	PASS