


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF051519\
Data File : VF062602.D
Acq On : 15 May 2019 9:48
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F051419S.M
Title : SW846 8260
Last Update : Wed May 15 05:06:28 2019

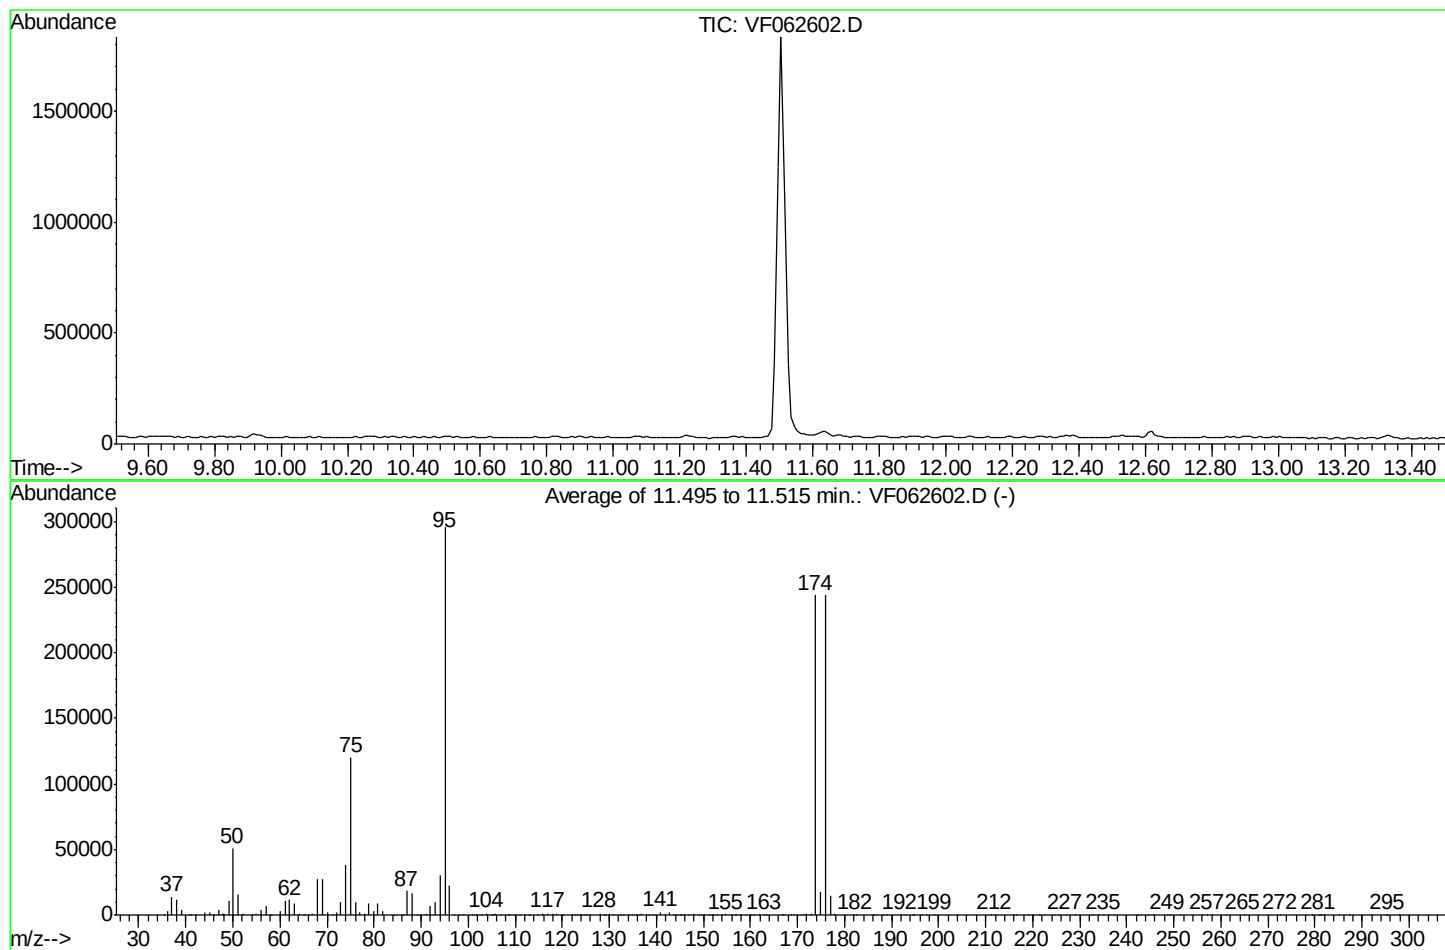

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	50543	PASS
75	95	30	60	40.5	119572	PASS
95	95	100	100	100.0	295530	PASS
96	95	5	9	7.5	22146	PASS
173	174	0.00	2	0.3	613	PASS
174	95	50	100	82.5	243797	PASS
175	174	5	9	7.2	17450	PASS
176	174	95	101	99.9	243626	PASS
177	176	5	9	6.1	14892	PASS