


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF051719\
Data File : VF062629.D
Acq On : 17 May 2019 9:28
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F051619S.M
Title : SW846 8260
Last Update : Fri May 17 05:49:09 2019

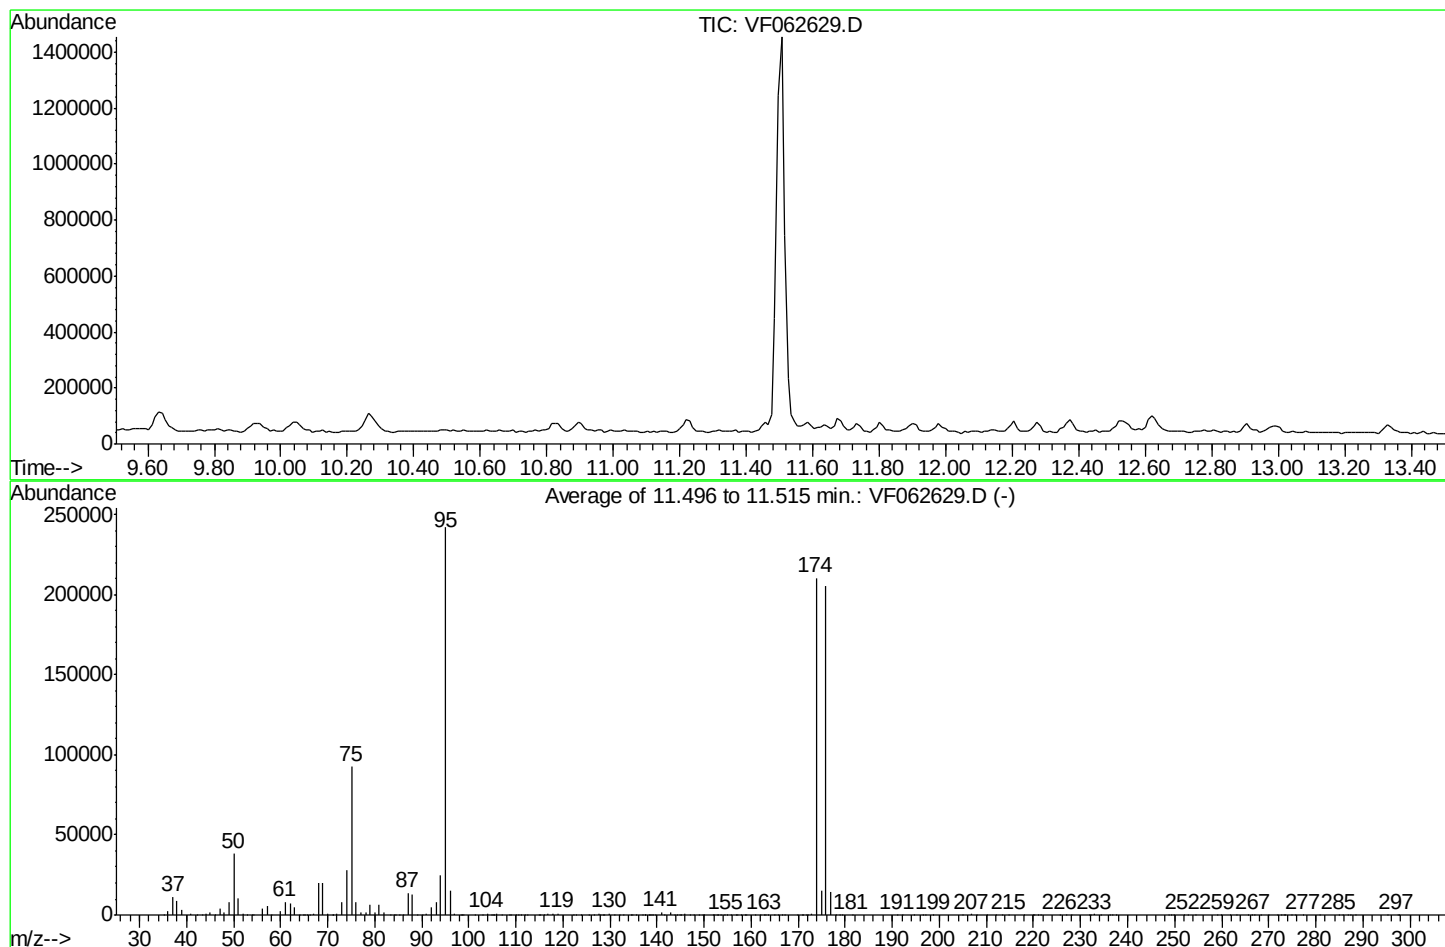

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	38037	PASS
75	95	30	60	38.3	92620	PASS
95	95	100	100	100.0	241926	PASS
96	95	5	9	6.1	14854	PASS
173	174	0.00	2	0.4	914	PASS
174	95	50	100	86.8	210090	PASS
175	174	5	9	7.3	15254	PASS
176	174	95	101	97.6	204949	PASS
177	176	5	9	6.9	14071	PASS