


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF052019\
 Data File : VF062651.D
 Acq On : 20 May 2019 9:53
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F051619S.M
 Title : SW846 8260
 Last Update : Fri May 17 05:49:09 2019

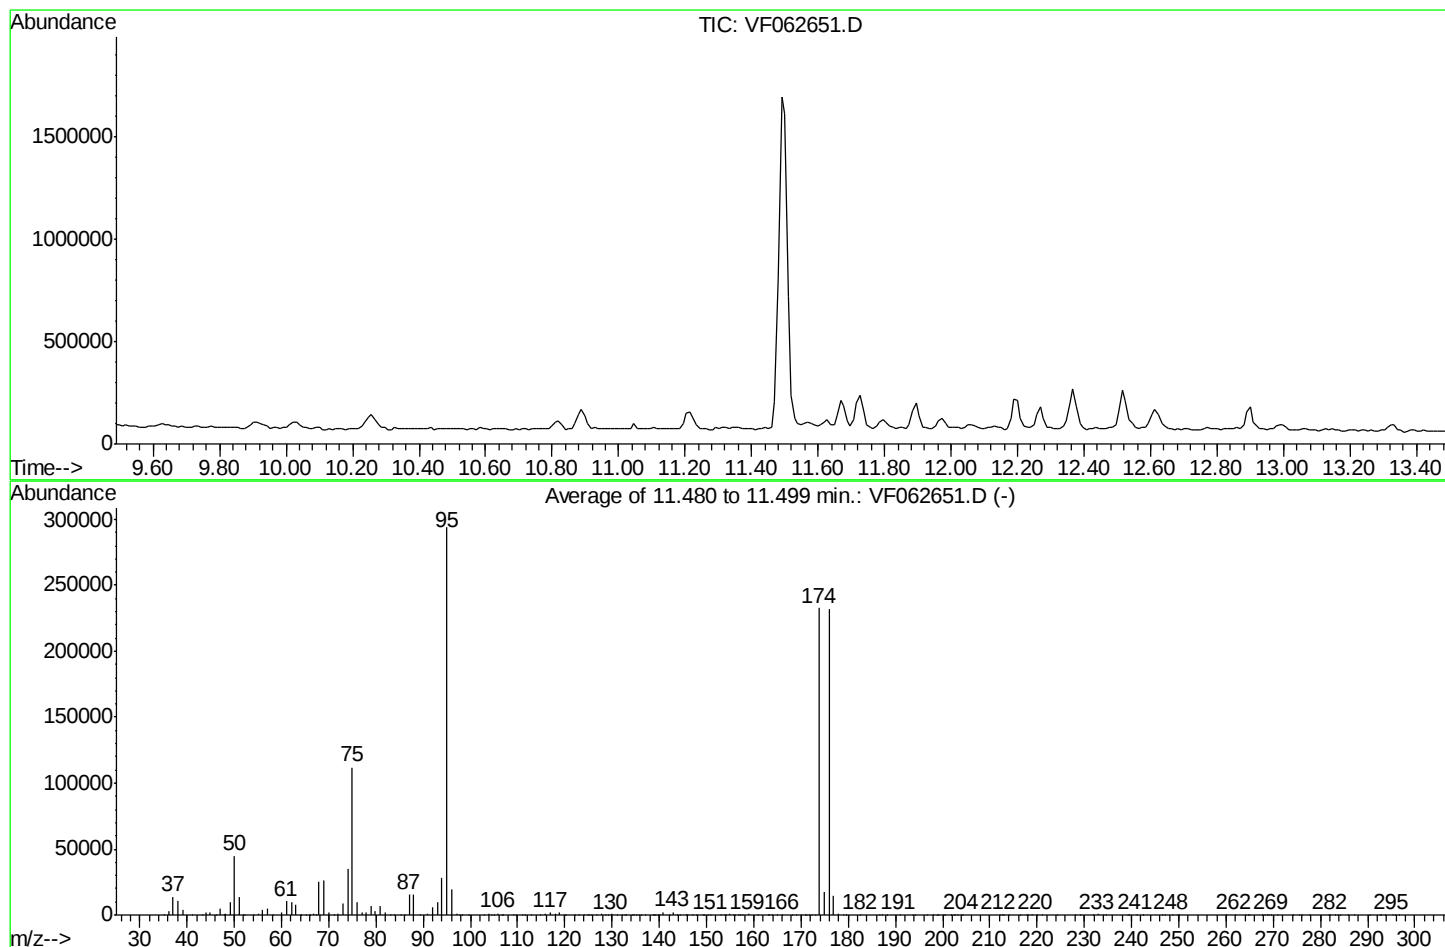

AutoFind: Scans 1110, 1111, 1112; Background Corrected with Scan 1104

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	44757	PASS
75	95	30	60	38.0	111658	PASS
95	95	100	100	100.0	293926	PASS
96	95	5	9	6.7	19691	PASS
173	174	0.00	2	0.2	526	PASS
174	95	50	100	79.1	232540	PASS
175	174	5	9	7.4	17303	PASS
176	174	95	101	99.6	231666	PASS
177	176	5	9	6.5	15072	PASS