


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF052319\
Data File : VF062718.D
Acq On : 23 May 2019 9:41
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F051619S.M
Title : SW846 8260
Last Update : Fri May 17 05:49:09 2019

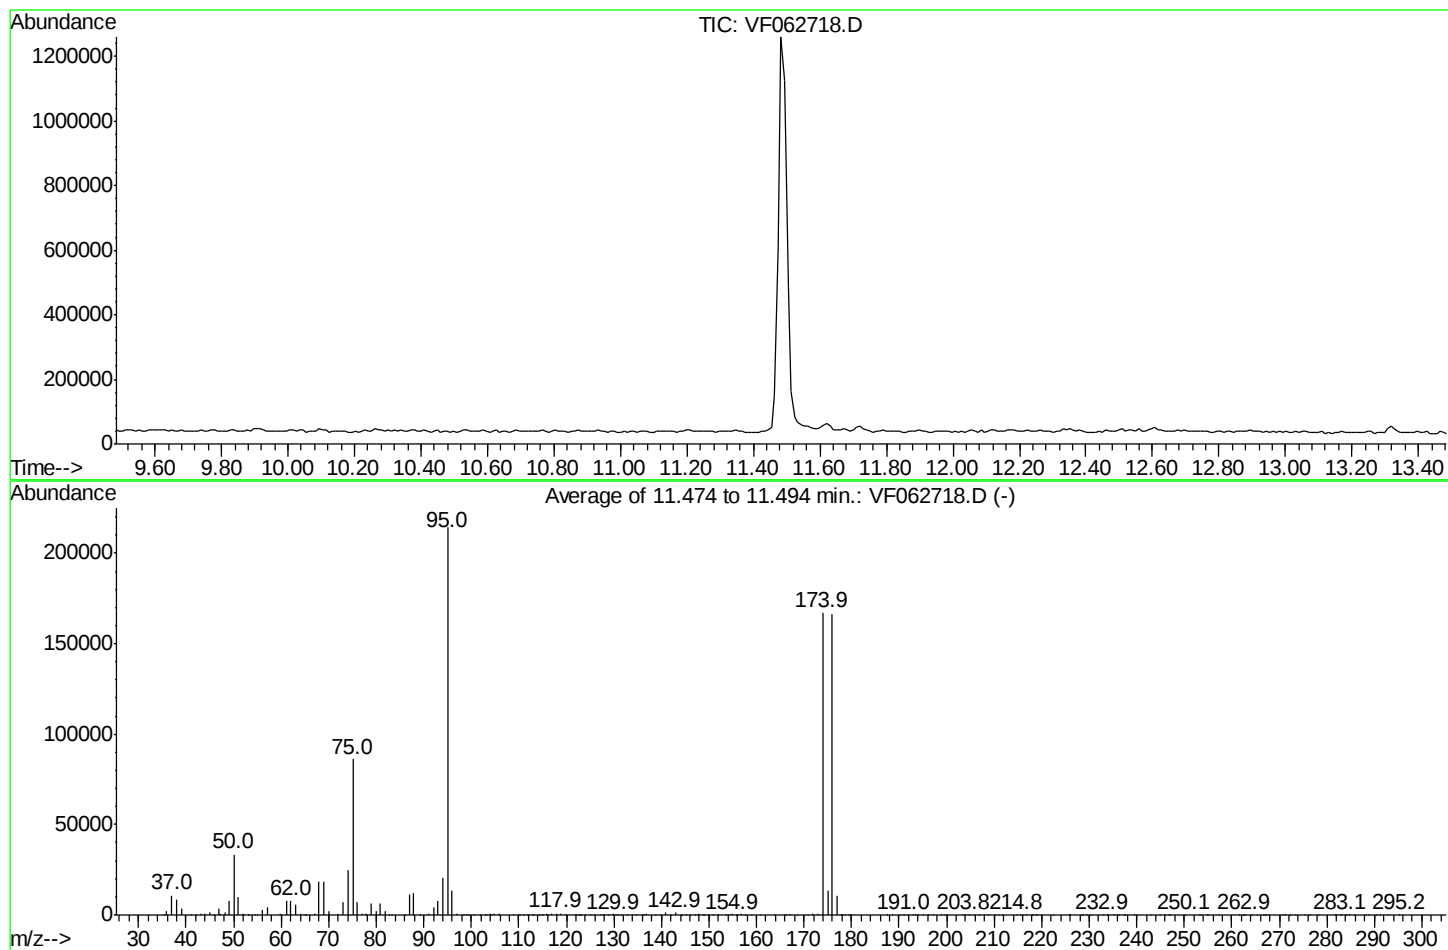

AutoFind: Scans 1110, 1111, 1112; Background Corrected with Scan 1103

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	33424	PASS
75	95	30	60	40.2	86229	PASS
95	95	100	100	100.0	214300	PASS
96	95	5	9	6.2	13359	PASS
173	174	0.00	2	0.3	563	PASS
174	95	50	100	78.1	167306	PASS
175	174	5	9	7.9	13167	PASS
176	174	95	101	99.2	166042	PASS
177	176	5	9	6.6	10882	PASS