

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF052819\
 Data File : VF062766.D
 Acq On : 28 May 2019 17:53
 Operator : FY/SY
 Sample : K3054-06
 Misc : 11.42g/5mL/MSVOA F/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 CULVER-CBTC-WC5A-052419

Quant Time: May 29 02:26:35 2019
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F051619S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 17 05:49:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.08	168	822834	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.80	114	1402139	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.93	117	1128611	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.63	152	455660	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.06	65	268678	46.21	ug/l	0.02
Spiked Amount	50.000		Recovery	=	92.42%	
35) Dibromofluoromethane	4.33	113	494893	46.13	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.26%	
50) Toluene-d8	7.73	98	1122166	43.81	ug/l	0.00
Spiked Amount	50.000		Recovery	=	87.62%	
62) 4-Bromofluorobenzene	11.51	95	404646	41.65	ug/l	0.00
Spiked Amount	50.000		Recovery	=	83.30%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF052819\
Data File : VF062766.D
Acq On : 28 May 2019 17:53
Operator : FY/SY
Sample : K3054-06
Misc : 11.42g/5mL/MSVOA F/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
CULVER-CBTC-WC5A-052419

Quant Time: May 29 02:26:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F051619S.M
Quant Title : SW846 8260
QLast Update : Fri May 17 05:49:09 2019
Response via : Initial Calibration

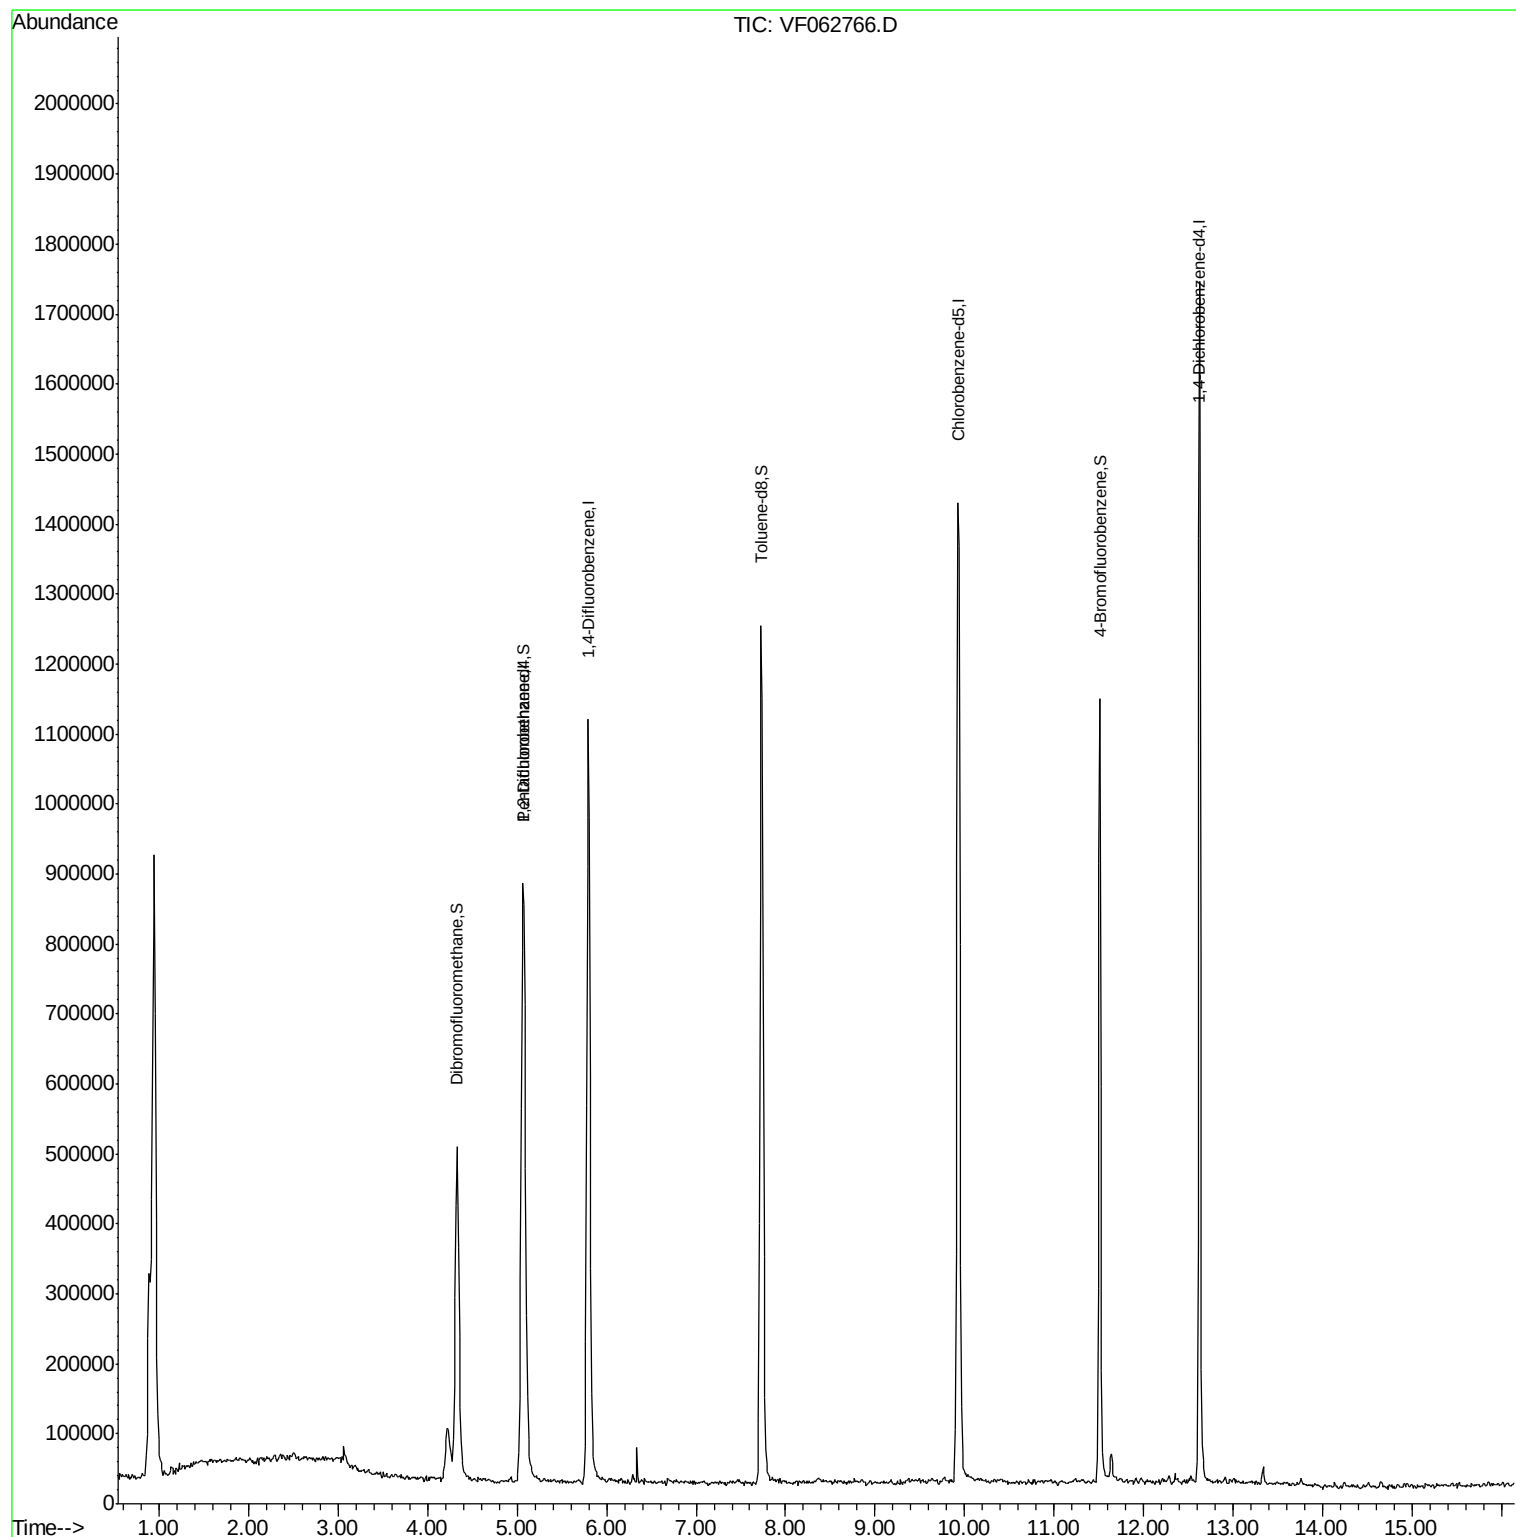

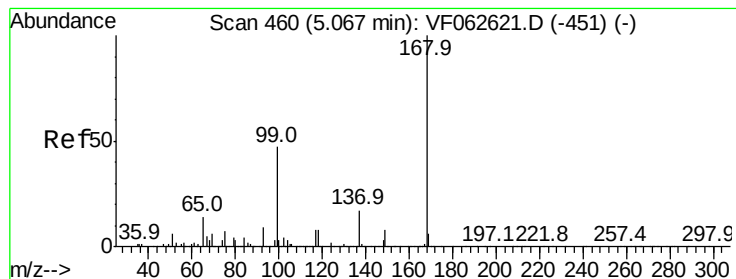

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.08 min Scan# 461

Delta R.T. 0.01 min

Lab File: VF062766.D

Acq: 28 May 2019 17:53

Instrument :

MSVOA_F

ClientSampleId :


CULVER-CBTC-WC5A-052419

Tot Ion:168 Resp: 822834

Ion Ratio Lower Upper

168 100

99 45.1 37.8 56.8

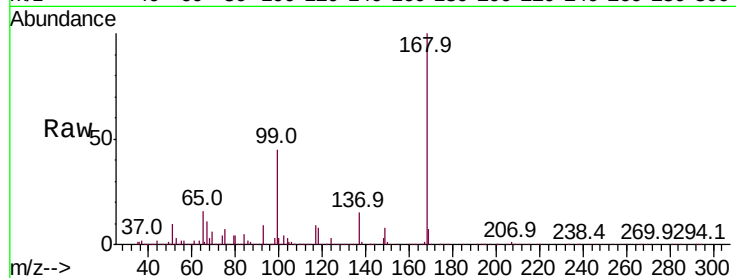

Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

5.08

250000

200000



150000

100000

50000

0

Time-->

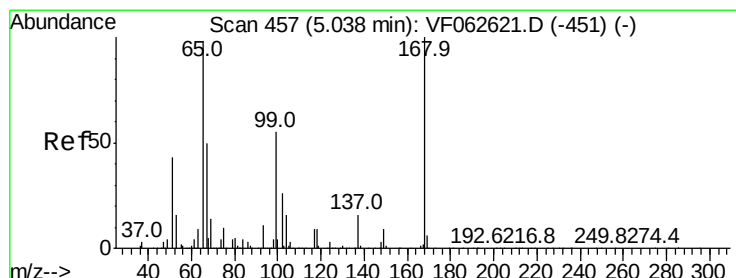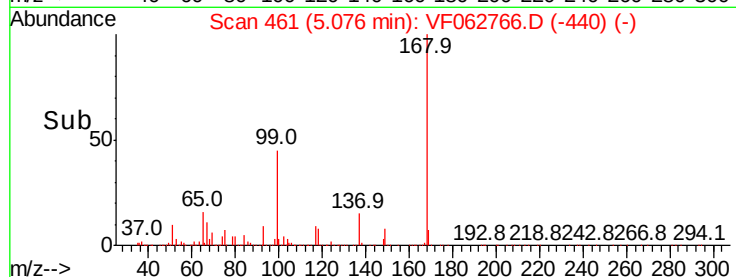

#33

1,2-Dichloroethane-d4

Concen: 46.208 ug/l

RT: 5.06 min Scan# 459

Delta R.T. 0.02 min

Lab File: VF062766.D


Acq: 28 May 2019 17:53

Tgt Ion: 65 Resp: 268678

Ion Ratio Lower Upper

65 100

67 56.0 0.0 117.6

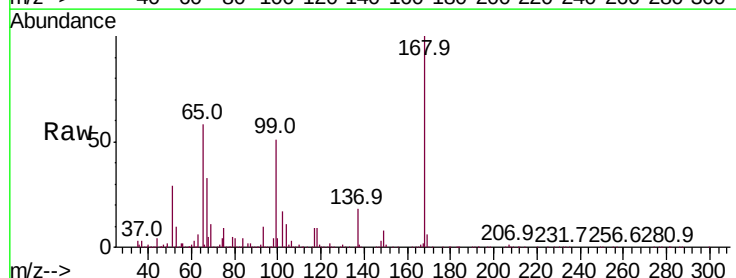

Abundance Ion 65.00 (64.70 to 65.70): VF0

Ion 67.00 (66.70 to 67.70): VF0

100000

80000


60000


40000

20000

0

Time-->

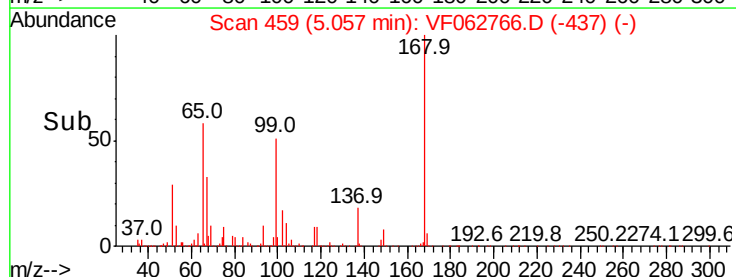

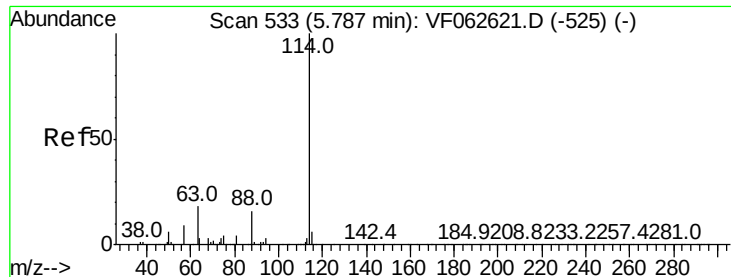

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.80 min Scan# 534

Delta R.T. 0.01 min

Lab File: VF062766.D

Acq: 28 May 2019 17:53

Instrument :

MSVOA_F

ClientSampleId :

CULVER-CBTC-WC5A-052419


Tot Ion:114 Resp: 1402139

Ion Ratio Lower Upper

114 100

63 17.0 0.0 35.4




88 16.5 0.0 32.4

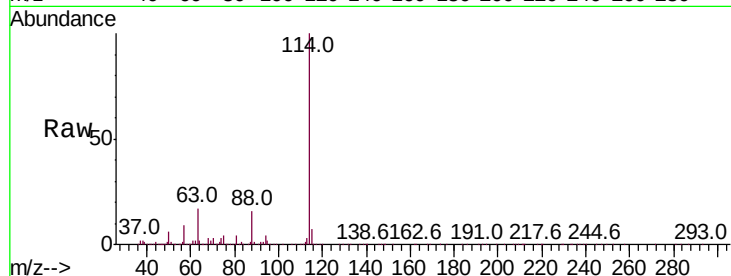

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 88.00 (87.70 to 88.70): VF0

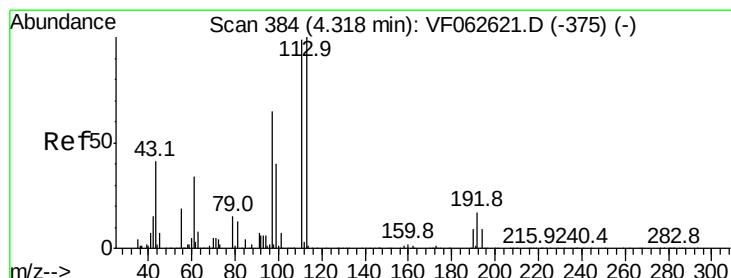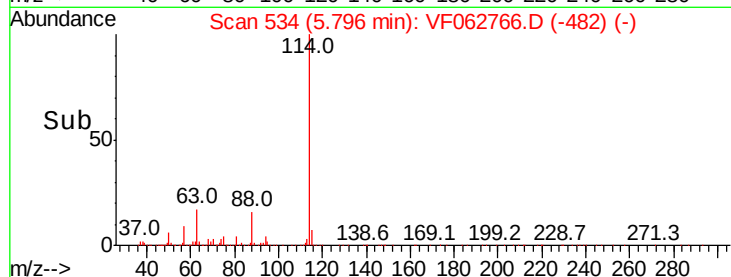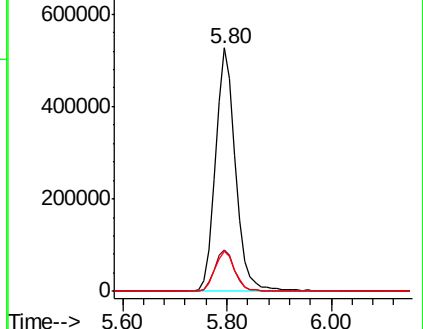

#35

Dibromofluoromethane

Concen: 46.126 ug/l

RT: 4.33 min Scan# 385

Delta R.T. 0.01 min

Lab File: VF062766.D

Acq: 28 May 2019 17:53


Tgt Ion:113 Resp: 494893

Ion Ratio Lower Upper

113 100

111 102.2 79.4 119.2



192 18.5 13.4 20.2

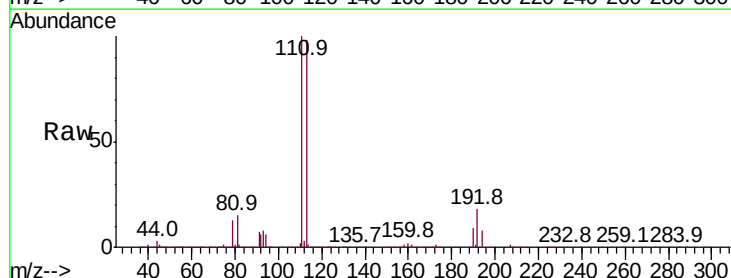


Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V



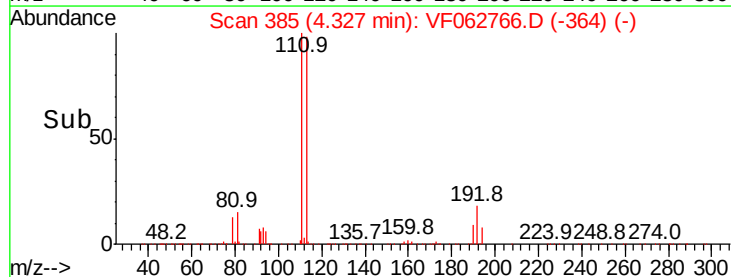
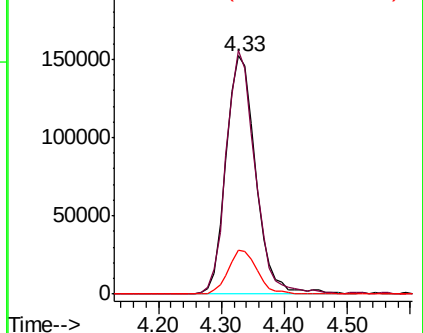


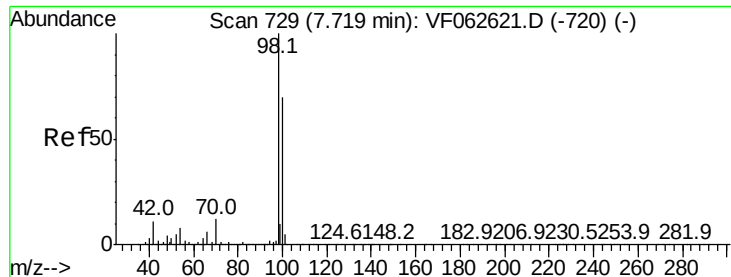

#50
Toluene-d8
Concen: 43.805 ug/l
RT: 7.73 min Scan# 730
Delta R.T. 0.01 min
Lab File: VF062766.D
Acq: 28 May 2019 17:53




Instrument :
MSVOA_F
ClientSampleId :
CULVER-CBTC-WC5A-052419


Tot Ion: 98 Resp: 1122166
Ion Ratio Lower Upper
98 100
100 70.7 56.2 84.2

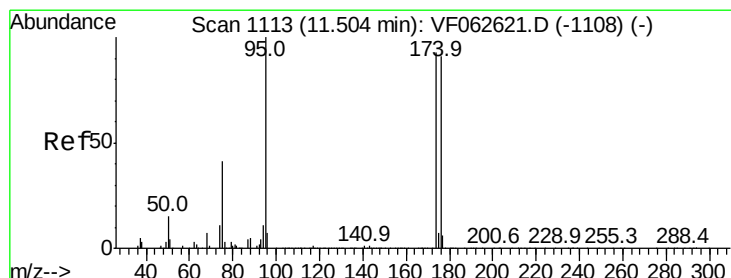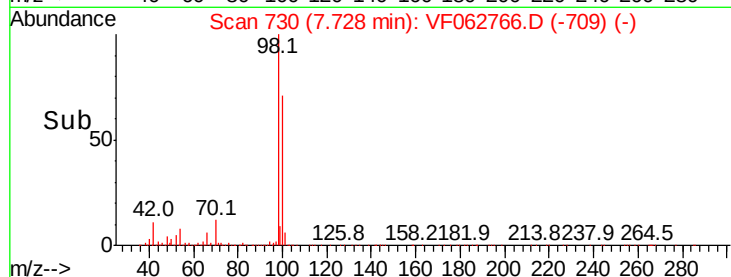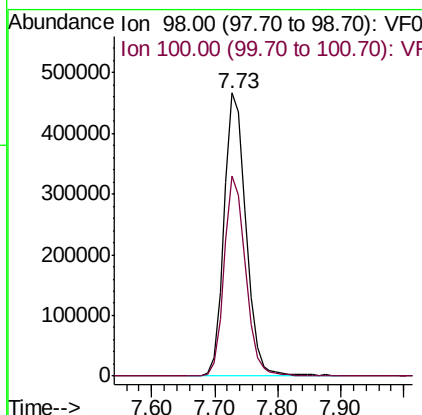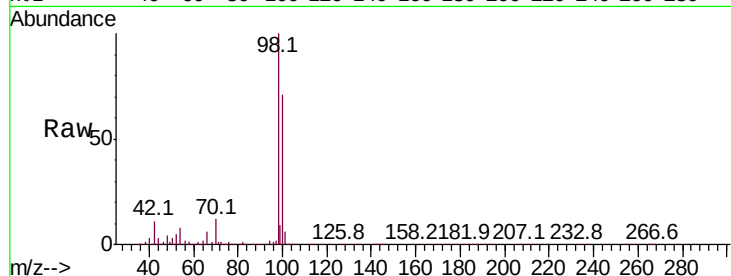

#62
4-Bromofluorobenzene
Concen: 41.648 ug/l
RT: 11.51 min Scan# 1114
Delta R.T. 0.01 min
Lab File: VF062766.D
Acq: 28 May 2019 17:53

Tgt Ion: 95 Resp: 404646
Ion Ratio Lower Upper
95 100
174 88.1 0.0 185.6
176 85.9 0.0 182.4


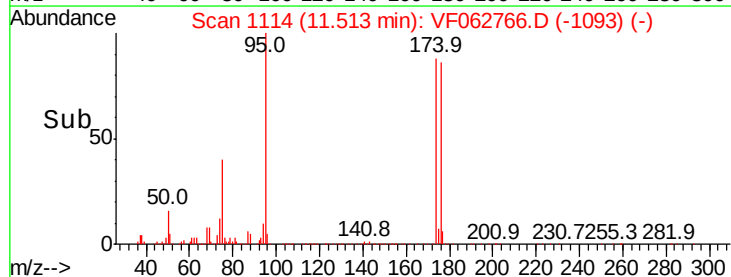
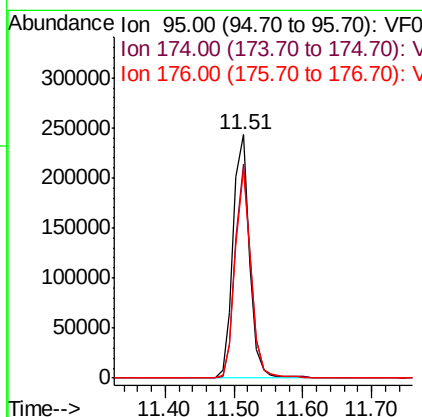
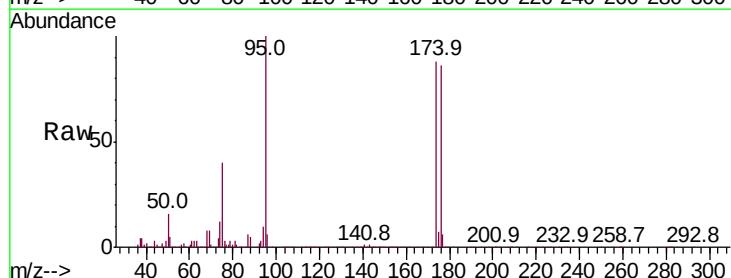


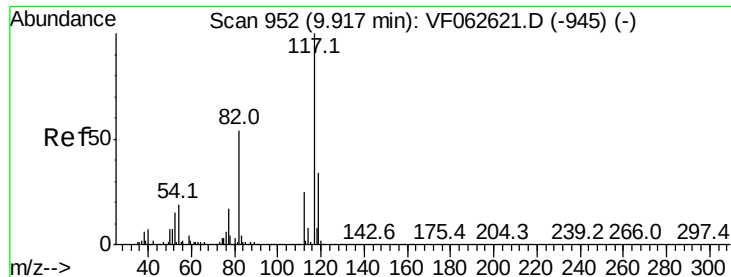

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.93 min Scan# 953
Delta R.T. 0.01 min
Lab File: VF062766.D
Acq: 28 May 2019 17:53

Instrument :
MSVOA_F
ClientSampleId :
CULVER-CBTC-WC5A-052419

Tot Ion:117 Resp: 1128611
Ion Ratio Lower Upper
117 100
82 55.5 43.3 64.9
119 33.6 27.4 41.0

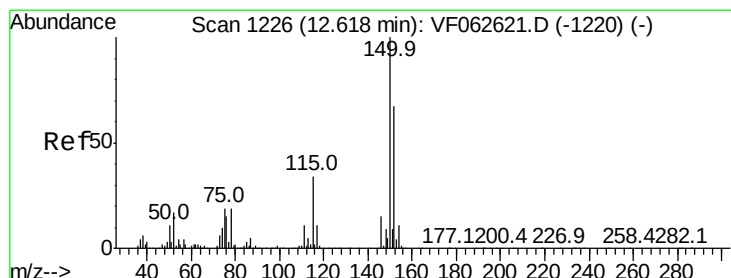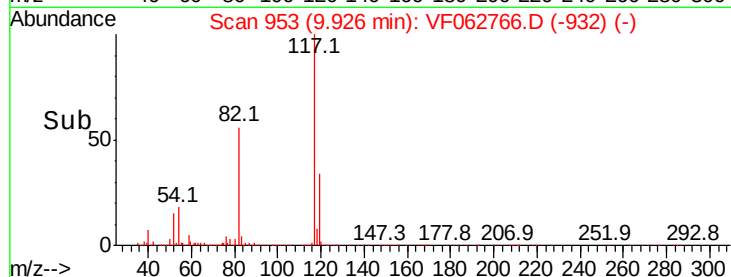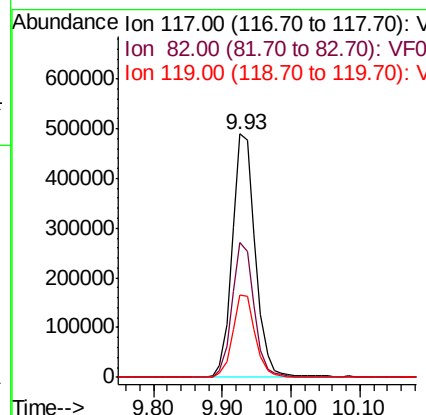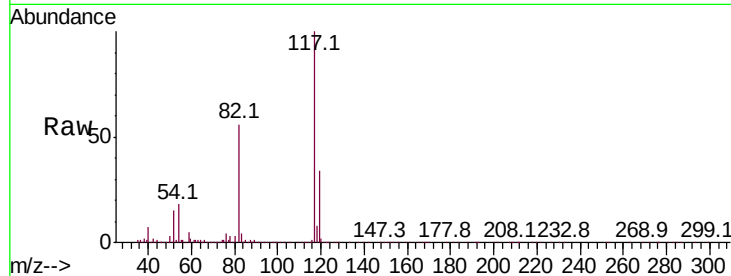

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.63 min Scan# 1227
Delta R.T. 0.01 min
Lab File: VF062766.D
Acq: 28 May 2019 17:53

Tgt Ion:152 Resp: 455660
Ion Ratio Lower Upper
152 100
115 51.6 25.2 75.6
150 147.7 0.0 306.2

