


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF052819\
Data File : VF062752.D
Acq On : 28 May 2019 9:40
Operator : FY/SY
Sample : BFB
Misc : 5.00g/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F051619S.M
Title : SW846 8260
Last Update : Fri May 17 05:49:09 2019

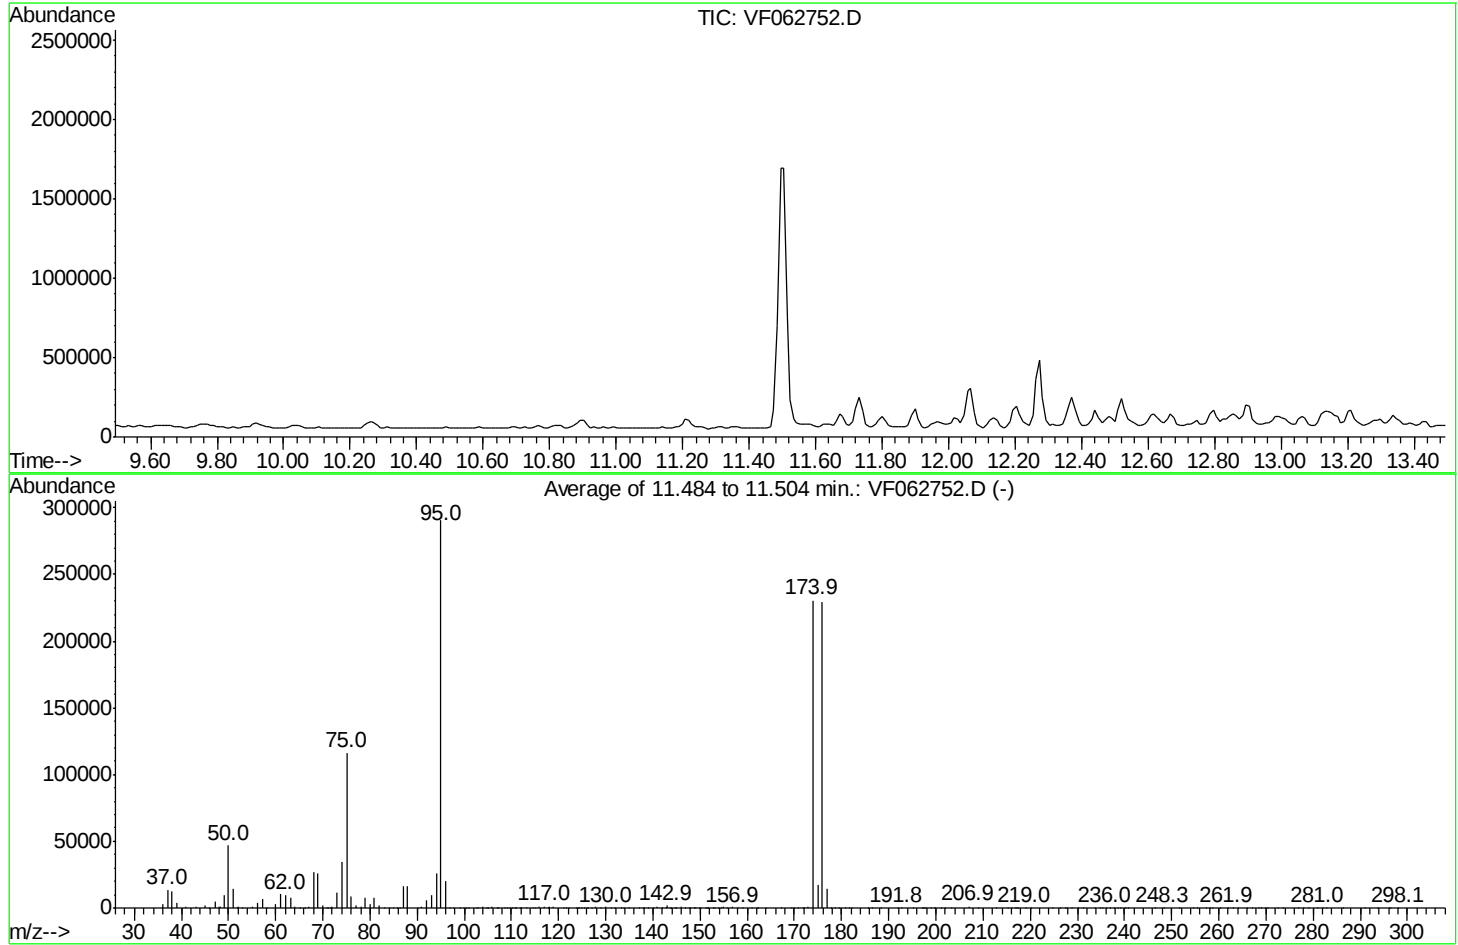

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	46654	PASS
75	95	30	60	40.1	116410	PASS
95	95	100	100	100.0	290582	PASS
96	95	5	9	7.0	20385	PASS
173	174	0.00	2	0.3	785	PASS
174	95	50	100	79.4	230664	PASS
175	174	5	9	7.3	16926	PASS
176	174	95	101	99.3	229152	PASS
177	176	5	9	6.4	14623	PASS