


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF052919\
 Data File : VF062773.D
 Acq On : 29 May 2019 9:47
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F051619S.M
 Title : SW846 8260
 Last Update : Fri May 17 05:49:09 2019

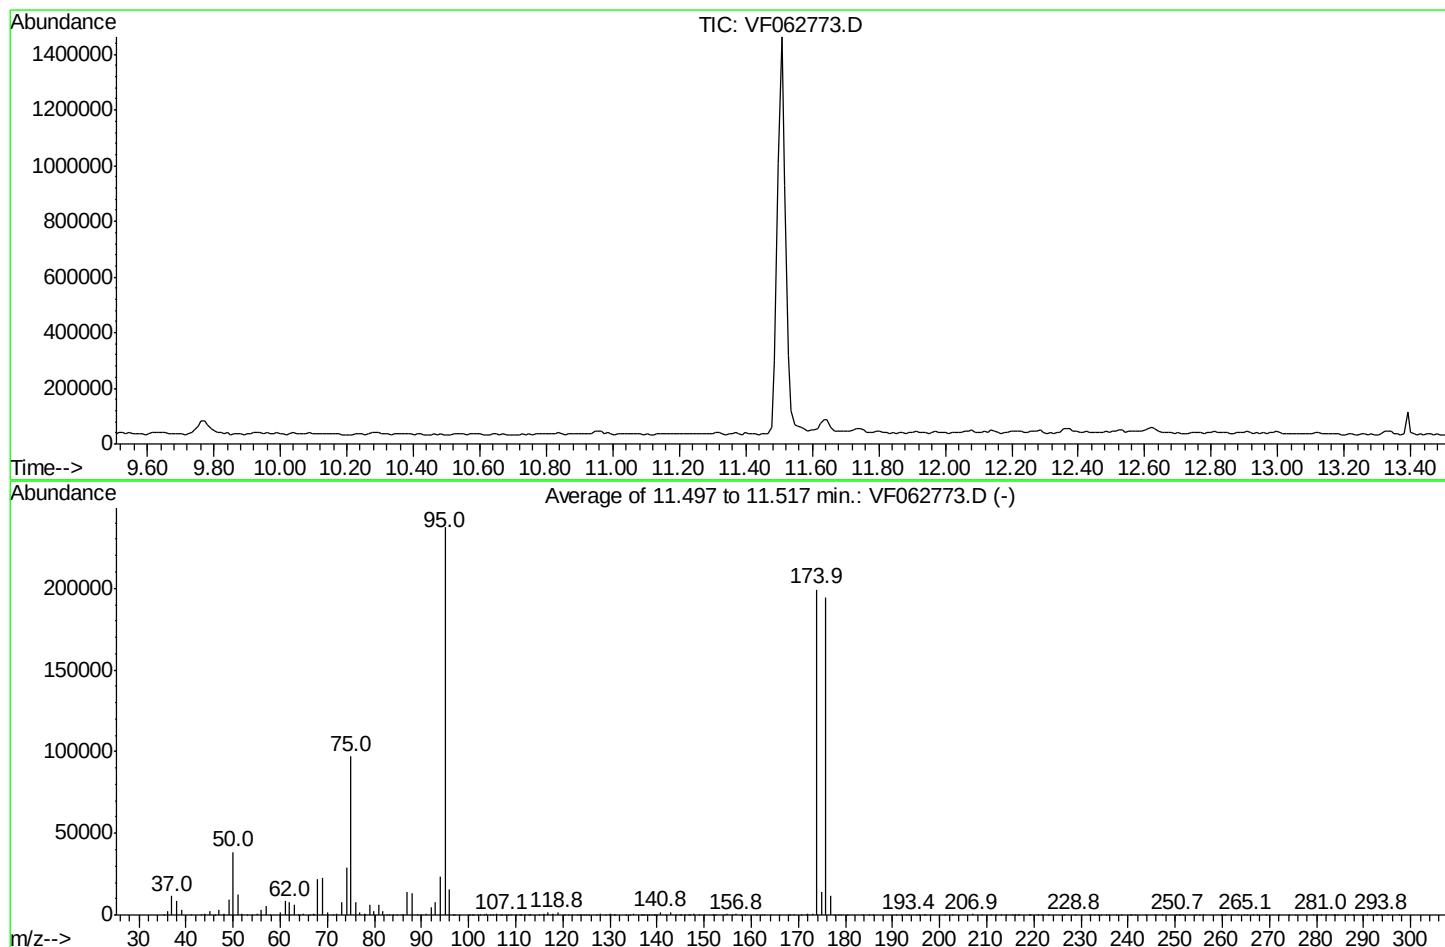

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	38472	PASS
75	95	30	60	40.8	96808	PASS
95	95	100	100	100.0	237280	PASS
96	95	5	9	6.6	15672	PASS
173	174	0.00	2	0.4	814	PASS
174	95	50	100	83.9	199018	PASS
175	174	5	9	7.1	14075	PASS
176	174	95	101	97.8	194581	PASS
177	176	5	9	5.9	11505	PASS