



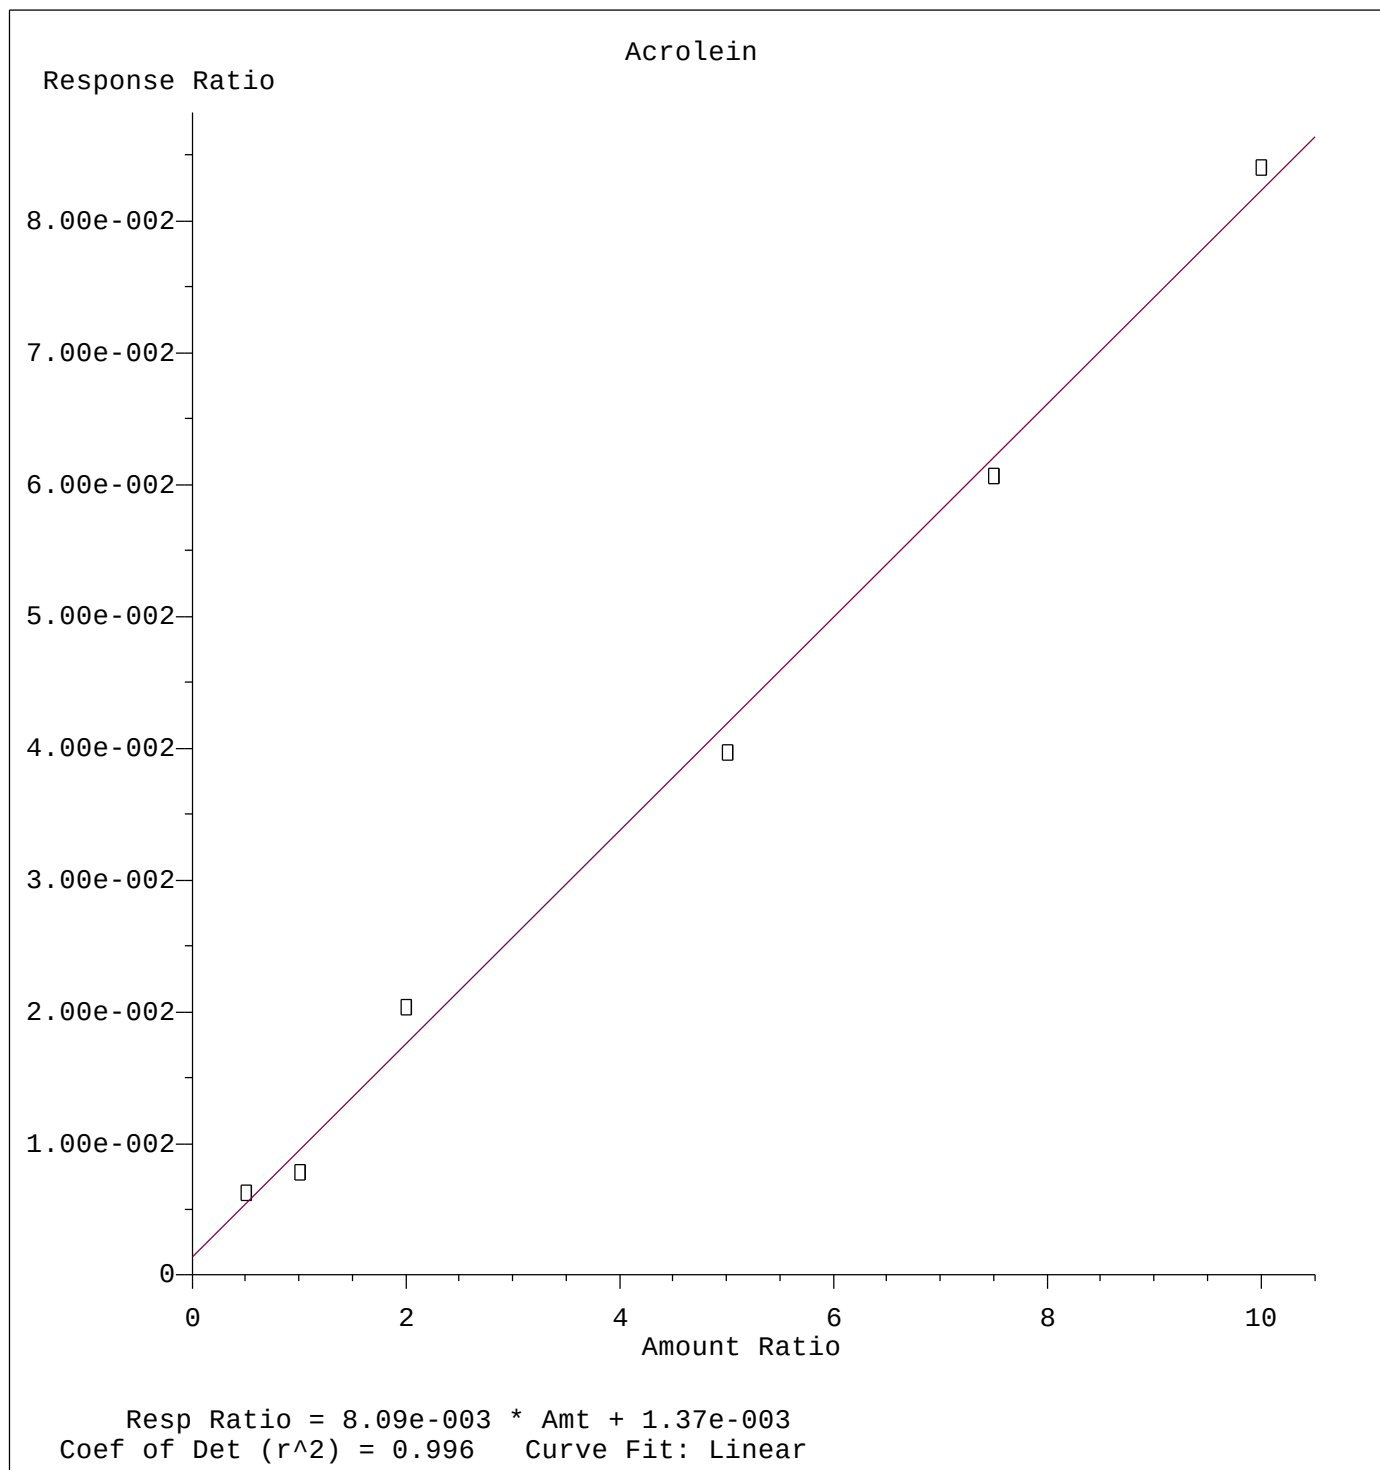


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F053019S.M
Calibration Table Last Updated: Fri May 31 04:18:30 2019

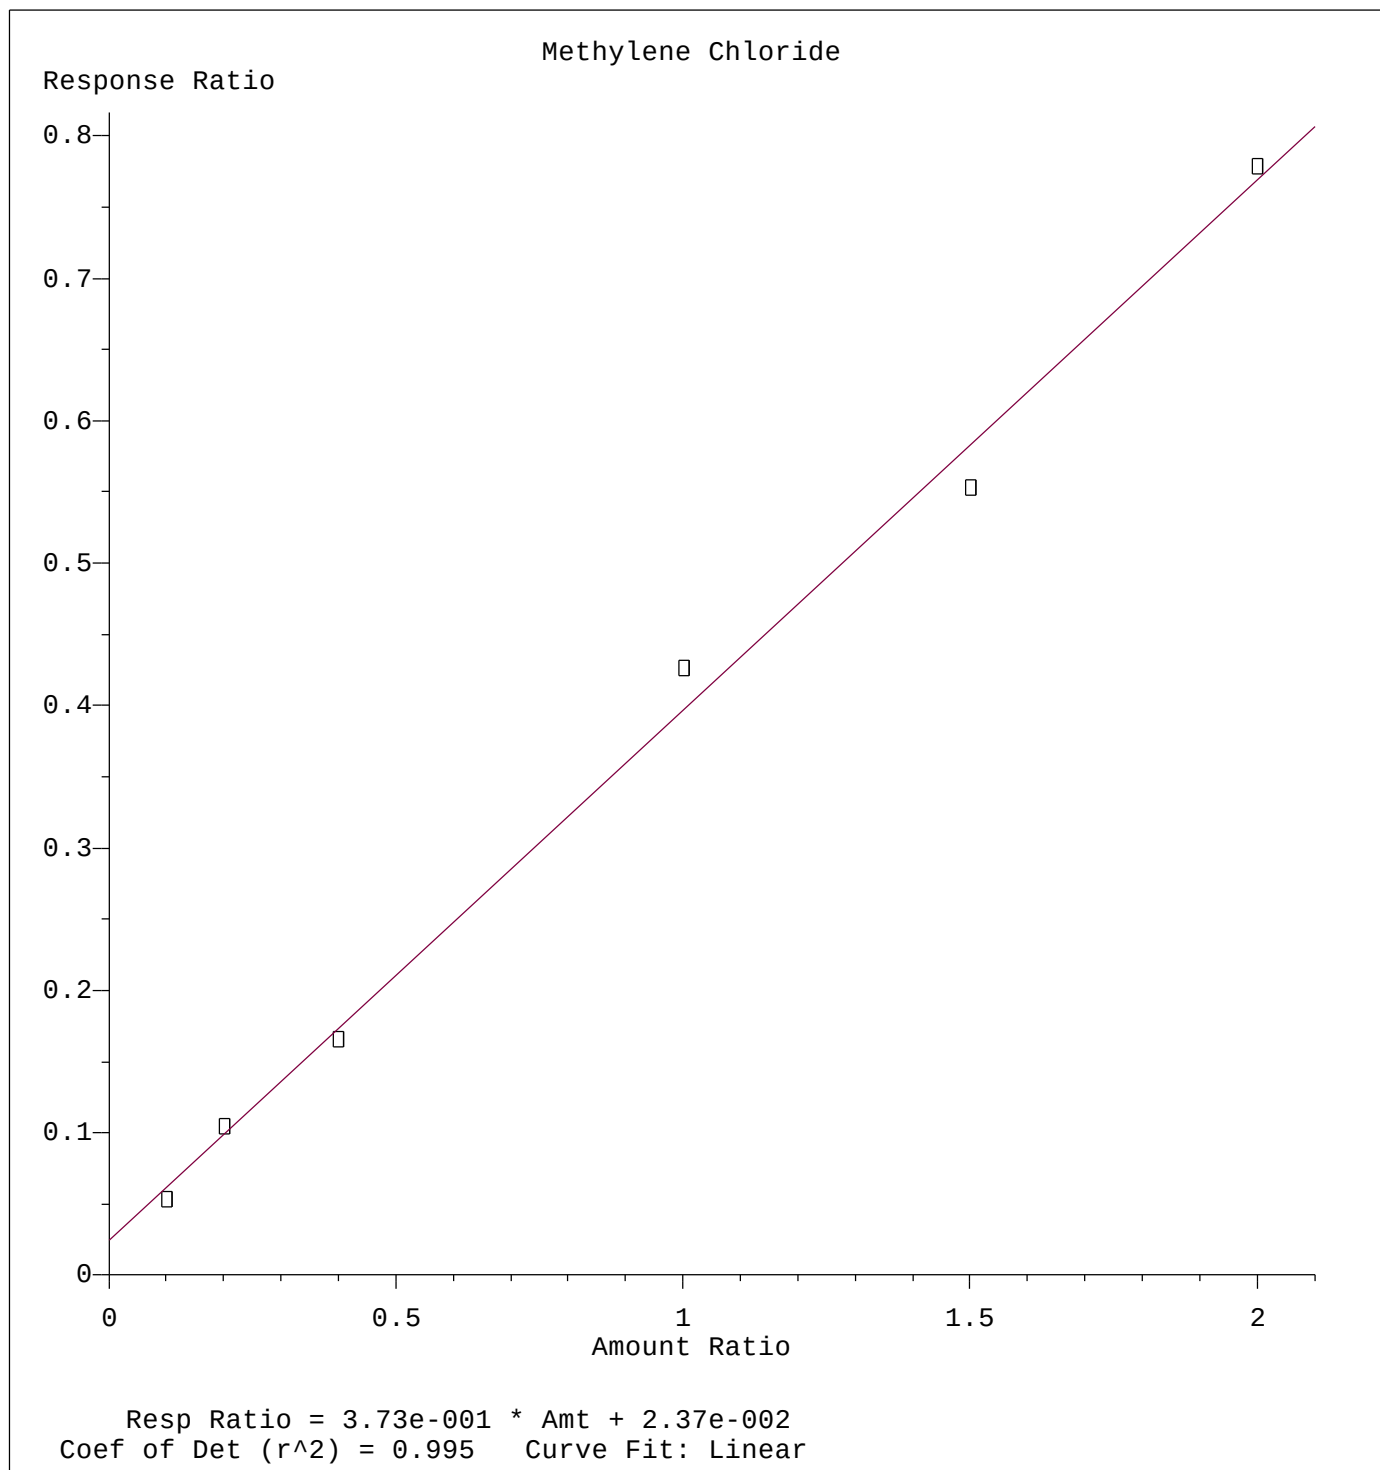

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F053019S.M
Calibration Table Last Updated: Fri May 31 04:18:30 2019

Dichlorodifluoromethane

Response Ratio

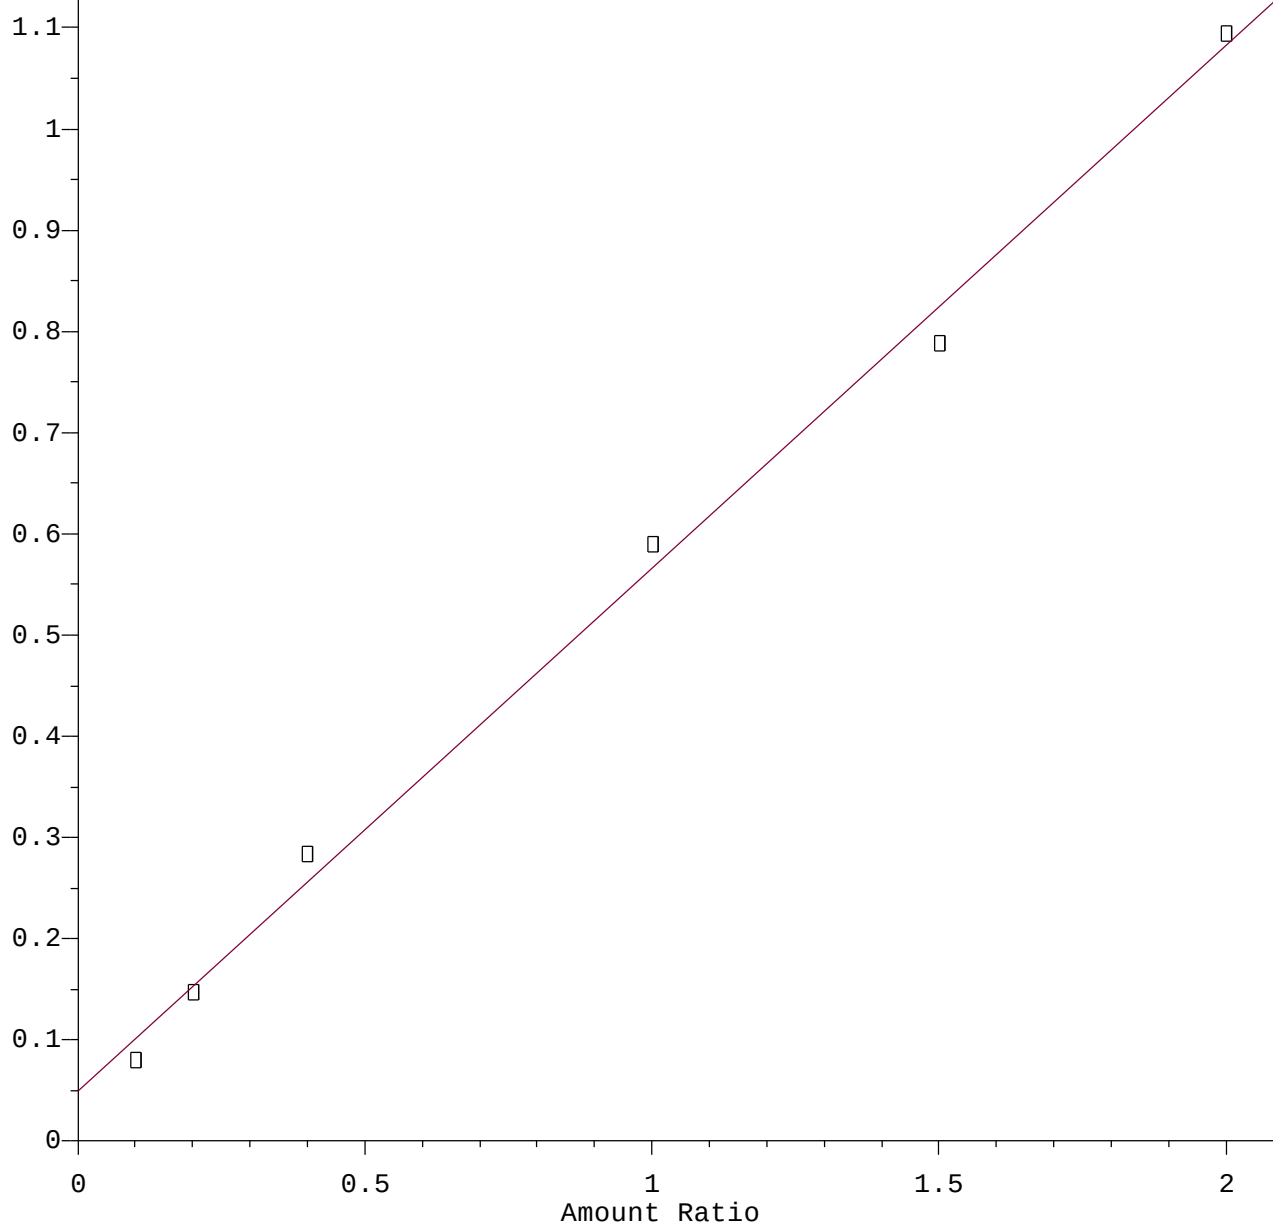

Resp Ratio = $5.17 \times 10^{-1} \times \text{Amt} + 4.87 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F053019S.M
Calibration Table Last Updated: Fri May 31 04:18:30 2019