


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF053019\  
Data File : VF062792.D  
Acq On : 30 May 2019 13:04  
Operator : FY/SY  
Sample : BFB  
Misc : 5.00µ/5mL/MSVOA F/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_F  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F053019S.M  
Title : SW846 8260  
Last Update : Fri May 31 04:18:30 2019

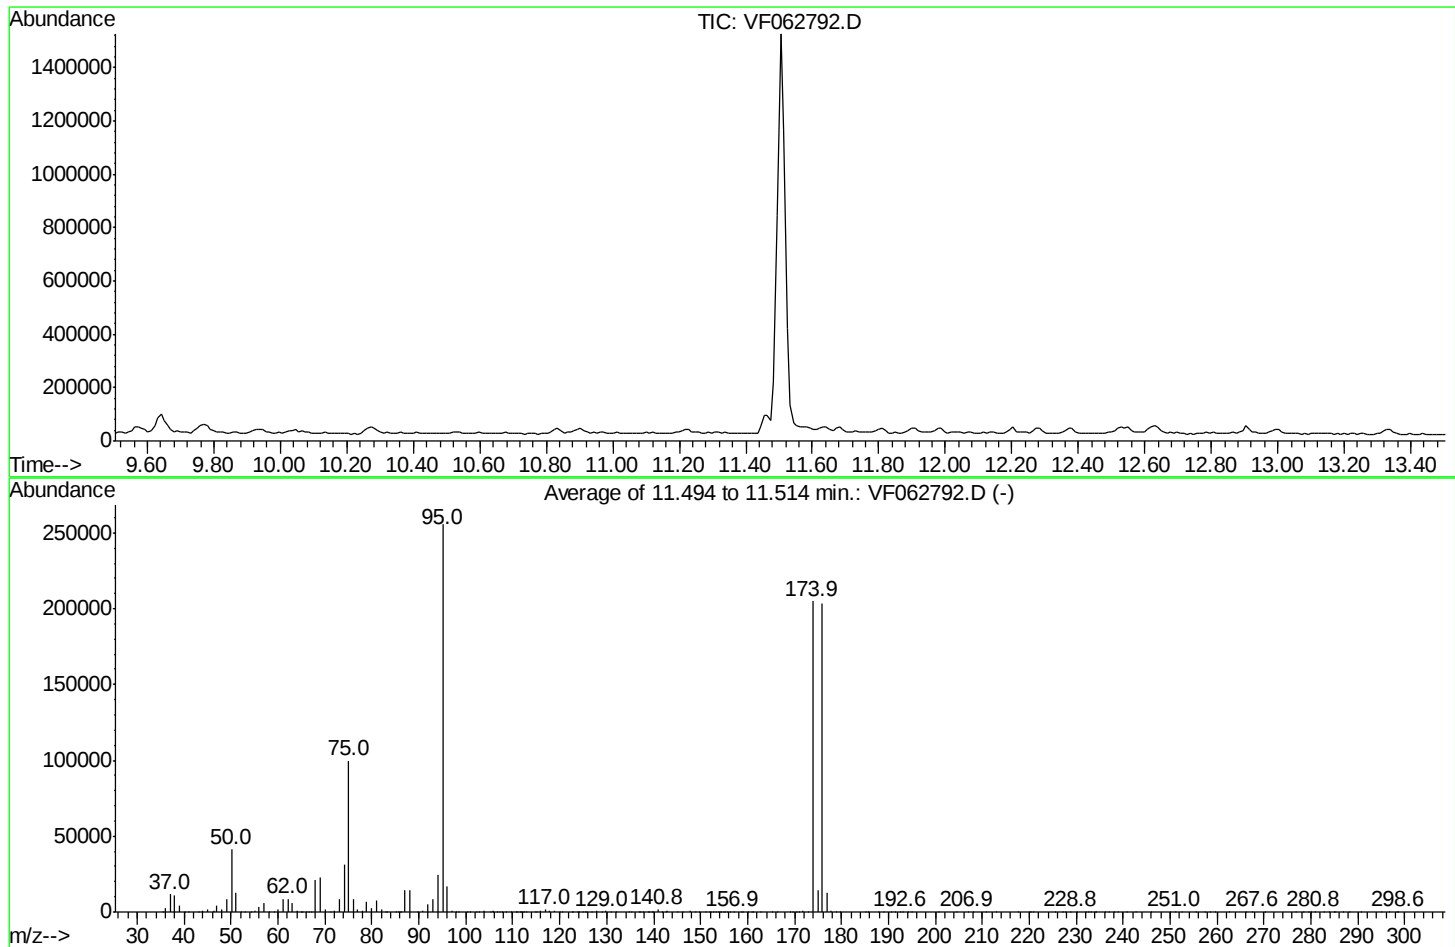

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.0      | 40981   | PASS             |
| 75          | 95           | 30           | 60           | 39.0      | 99765   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 255637  | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 16801   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.2       | 446     | PASS             |
| 174         | 95           | 50           | 100          | 80.2      | 205053  | PASS             |
| 175         | 174          | 5            | 9            | 6.8       | 14034   | PASS             |
| 176         | 174          | 95           | 101          | 99.1      | 203112  | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 12801   | PASS             |