


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF060319\
 Data File : VF062820.D
 Acq On : 3 Jun 2019 9:40
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F053019S.M
 Title : SW846 8260
 Last Update : Fri May 31 04:18:30 2019

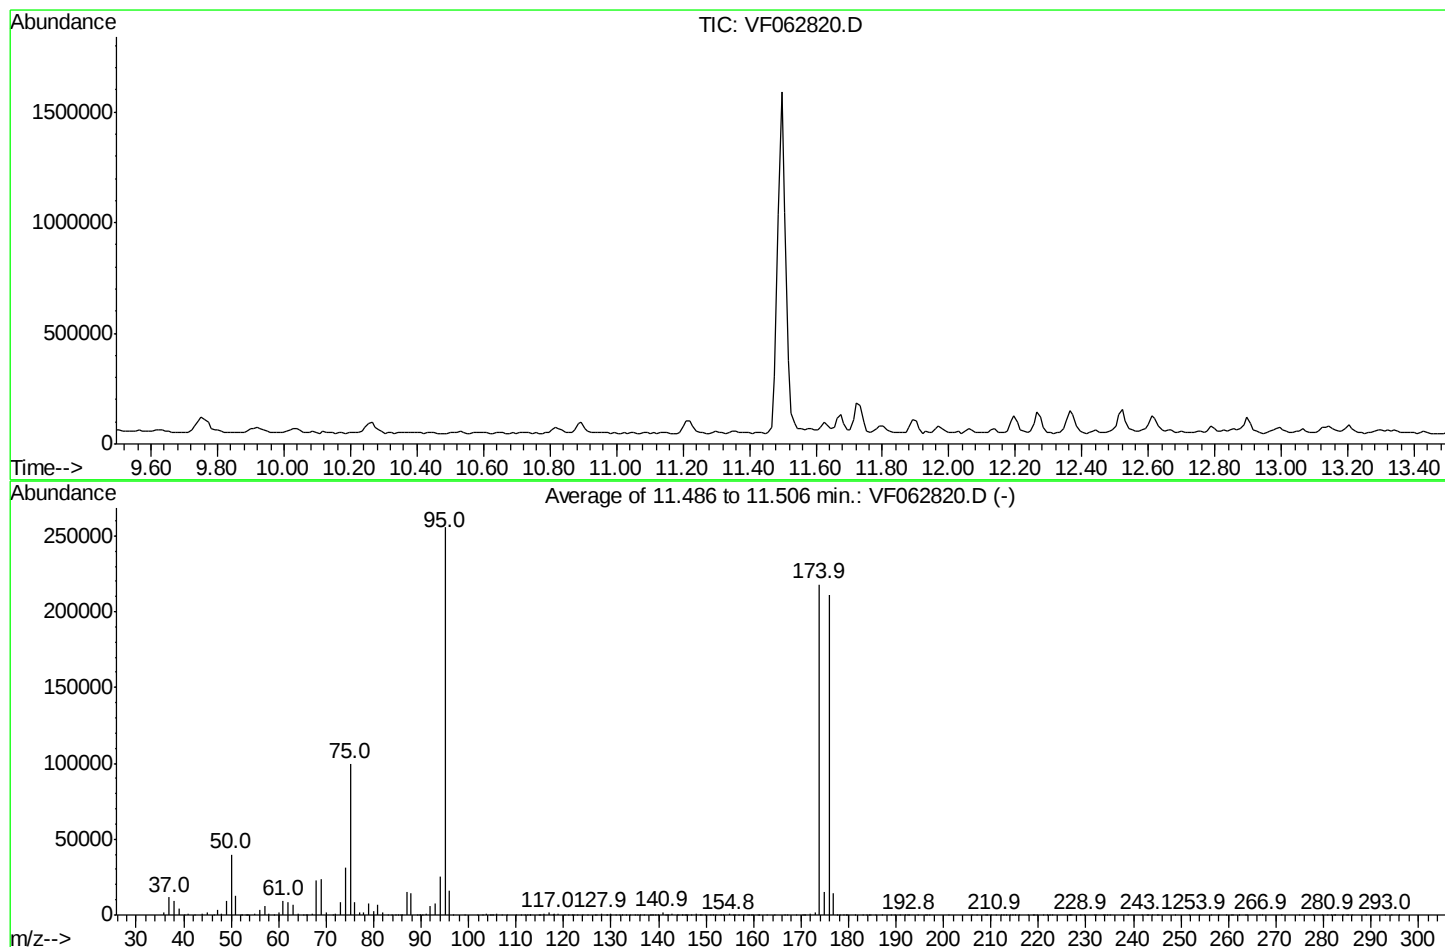

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1104

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	39984	PASS
75	95	30	60	39.1	99854	PASS
95	95	100	100	100.0	255667	PASS
96	95	5	9	6.4	16294	PASS
173	174	0.00	2	0.7	1445	PASS
174	95	50	100	85.4	218218	PASS
175	174	5	9	7.2	15642	PASS
176	174	95	101	96.9	211498	PASS
177	176	5	9	6.7	14102	PASS