


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF060419\  
 Data File : VF062835.D  
 Acq On : 4 Jun 2019 12:41  
 Operator : FY/SY  
 Sample : BFB  
 Misc : 5.00µ/5mL/MSVOA F/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_F  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F053019S.M  
 Title : SW846 8260  
 Last Update : Fri May 31 04:18:30 2019

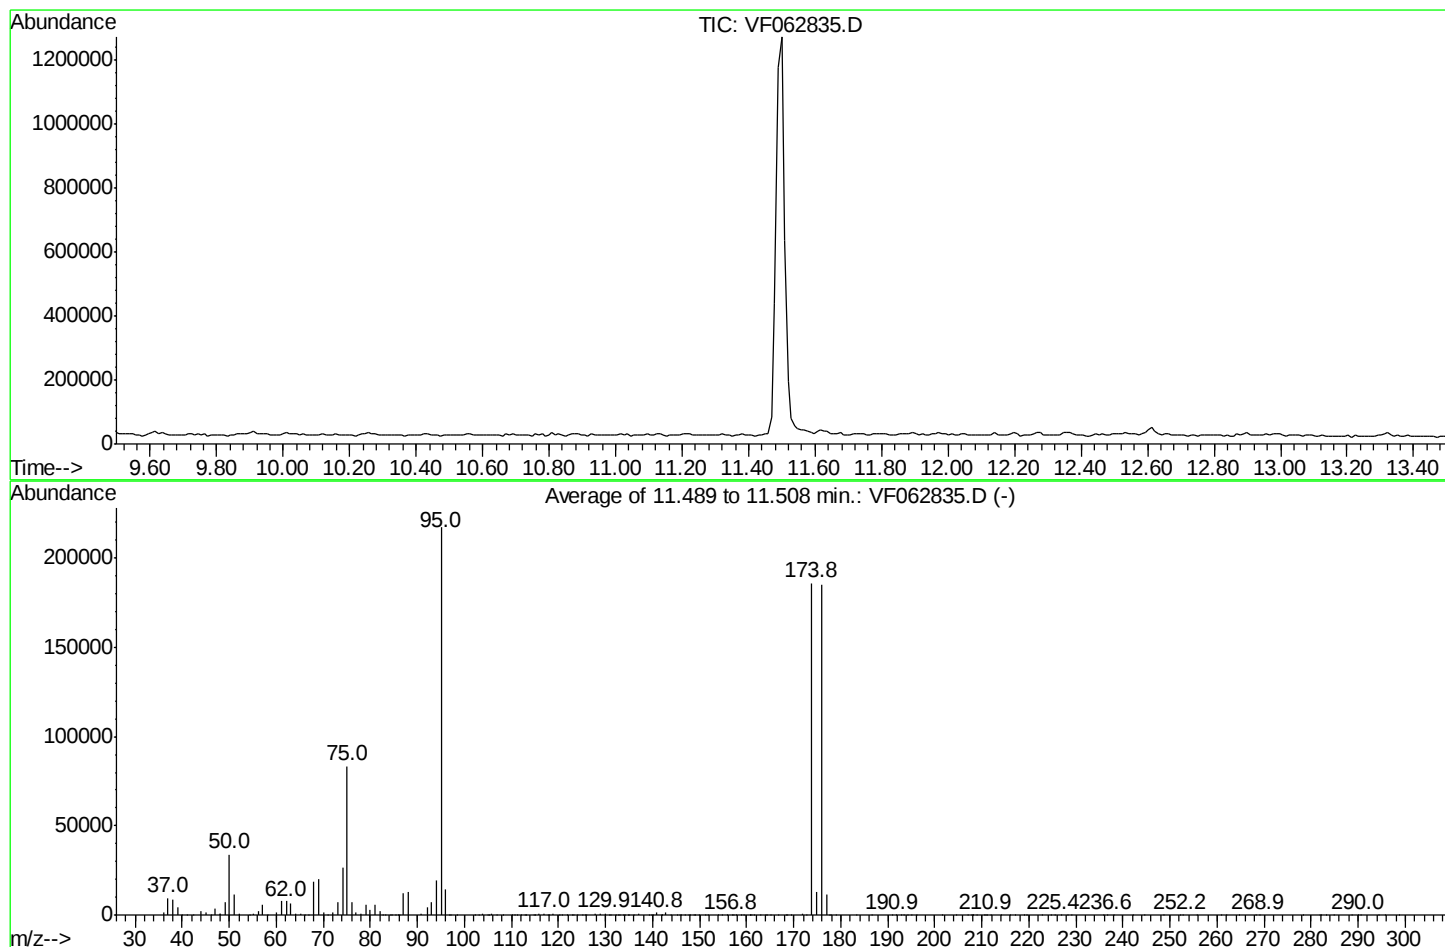

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1105

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.6      | 33927   | PASS             |
| 75          | 95           | 30           | 60           | 38.5      | 83571   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 217346  | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 14238   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.2       | 322     | PASS             |
| 174         | 95           | 50           | 100          | 85.6      | 185984  | PASS             |
| 175         | 174          | 5            | 9            | 7.0       | 13030   | PASS             |
| 176         | 174          | 95           | 101          | 99.4      | 184960  | PASS             |
| 177         | 176          | 5            | 9            | 6.2       | 11435   | PASS             |