


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060519\
Data File : BF114822.D
Acq On : 5 Jun 2019 17:09
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060419.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 04 16:57:15 2019

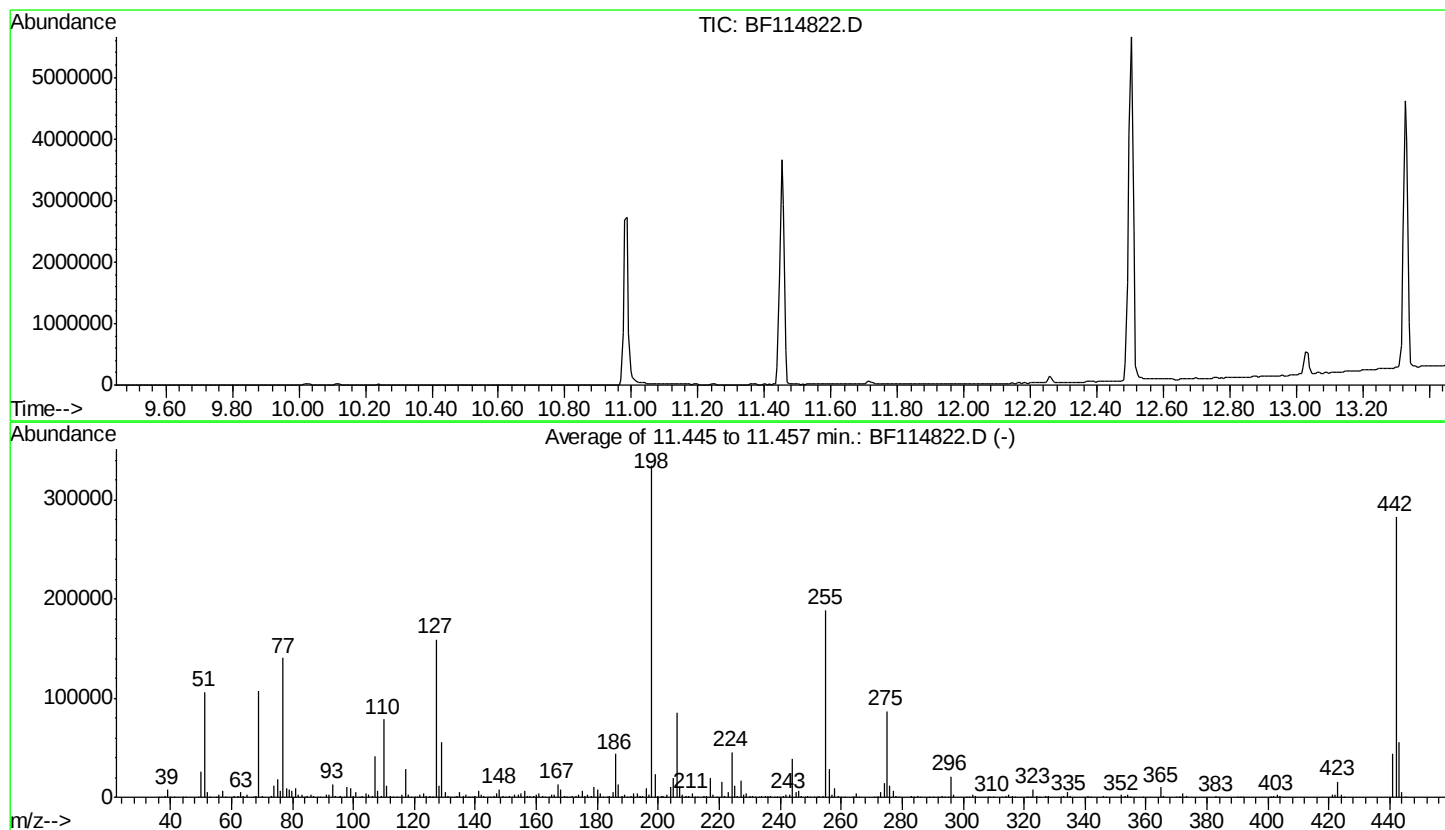

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	106384	PASS
68	69	0.00	2	1.3	1398	PASS
69	198	0.00	100	32.0	107100	PASS
70	69	0.00	2	0.7	771	PASS
127	198	10	80	47.6	159114	PASS
197	198	0.00	2	0.7	2292	PASS
198	198	100	100	100.0	334229	PASS
199	198	5	9	6.8	22832	PASS
275	198	10	60	25.9	86528	PASS
365	198	1	100	2.9	9859	PASS
441	198	0.01	100	13.3	44304	PASS
442	198	50	100	84.6	282714	PASS
443	442	15	24	19.8	55981	PASS