


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF060618\
 Data File : VF058108.D
 Acq On : 6 Jun 2018 15:14
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F060618S.M
 Title : SW846 8260
 Last Update : Thu Jun 07 10:52:00 2018

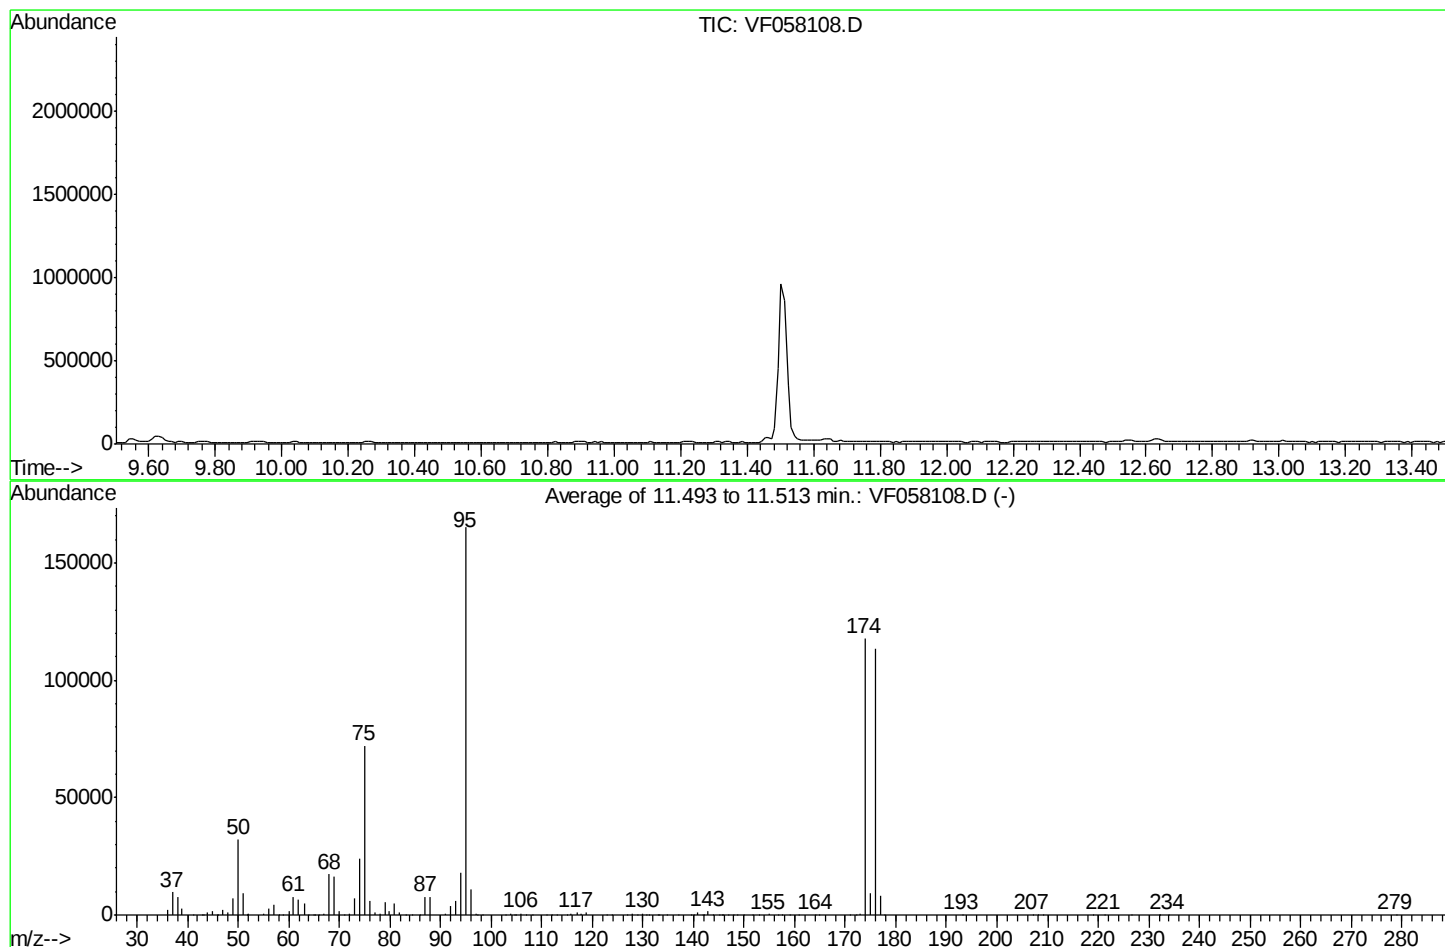

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	31981	PASS
75	95	30	60	43.6	72091	PASS
95	95	100	100	100.0	165176	PASS
96	95	5	9	6.7	11056	PASS
173	174	0.00	2	0.4	484	PASS
174	95	50	100	71.3	117781	PASS
175	174	5	9	7.8	9205	PASS
176	174	95	101	96.5	113685	PASS
177	176	5	9	7.1	8049	PASS