


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF060619\
 Data File : VF062874.D
 Acq On : 6 Jun 2019 9:37
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00q/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F053019S.M
 Title : SW846 8260
 Last Update : Fri May 31 04:18:30 2019

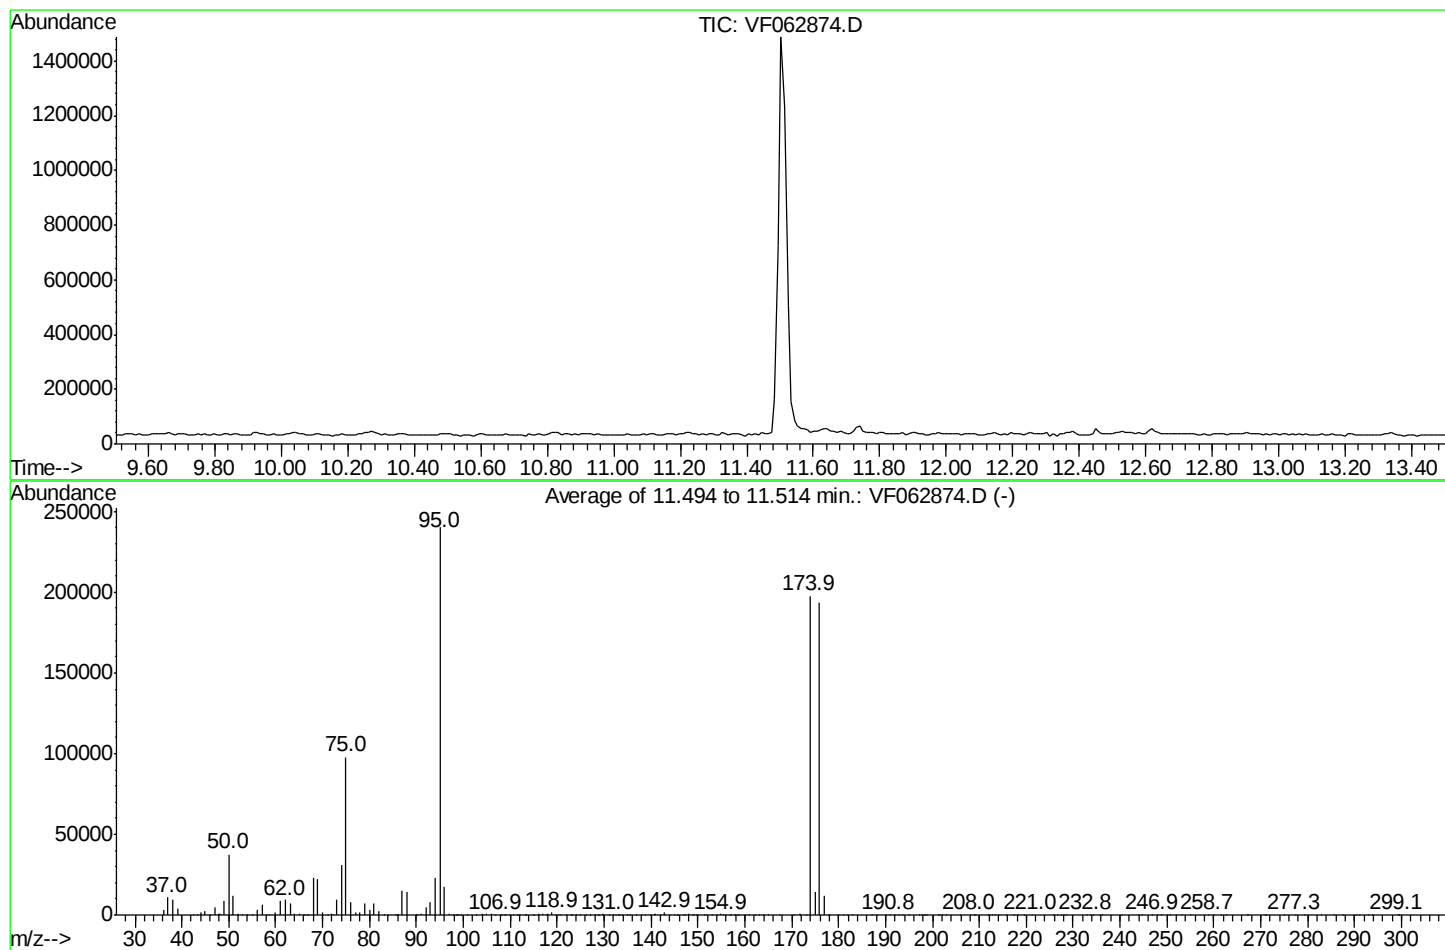

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1103

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	37566	PASS
75	95	30	60	40.7	97795	PASS
95	95	100	100	100.0	240192	PASS
96	95	5	9	7.3	17607	PASS
173	174	0.00	2	0.1	268	PASS
174	95	50	100	82.3	197784	PASS
175	174	5	9	7.4	14696	PASS
176	174	95	101	98.0	193741	PASS
177	176	5	9	6.3	12225	PASS