


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF061219\
Data File : VF062919.D
Acq On : 12 Jun 2019 9:38
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F053019S.M
Title : SW846 8260
Last Update : Fri May 31 04:18:30 2019

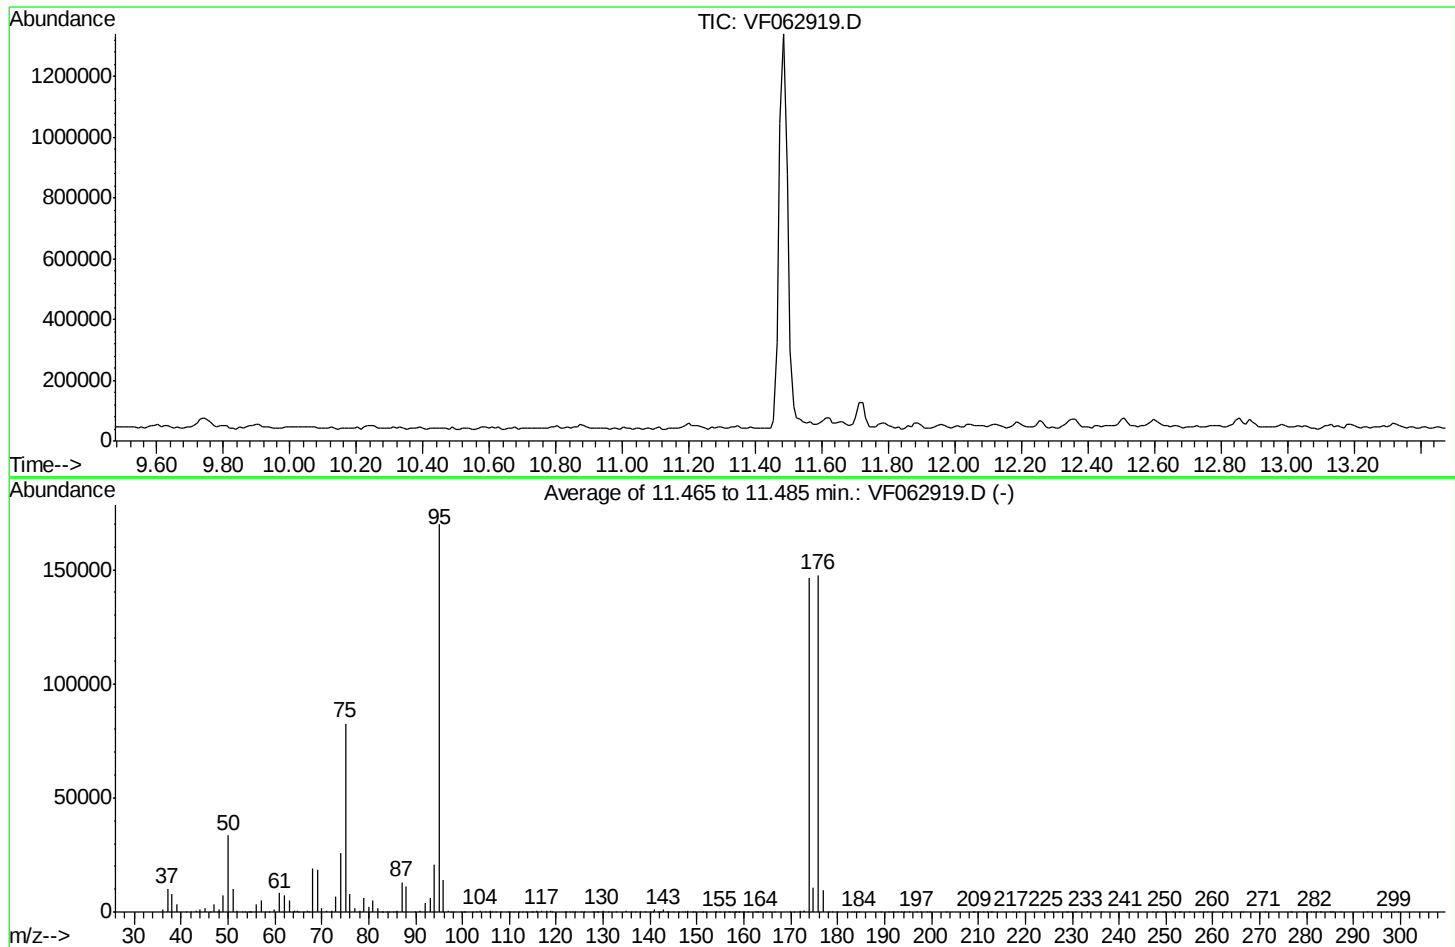

AutoFind: Scans 1109, 1110, 1111; Background Corrected with Scan 1104

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	33497	PASS
75	95	30	60	48.5	82452	PASS
95	95	100	100	100.0	169842	PASS
96	95	5	9	8.2	13900	PASS
173	174	0.00	2	0.4	640	PASS
174	95	50	100	86.1	146301	PASS
175	174	5	9	7.3	10716	PASS
176	174	95	101	100.8	147522	PASS
177	176	5	9	6.4	9479	PASS