


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF062618\
 Data File : VF059309.D
 Acq On : 26 Jun 2018 9:42
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F062518S.M
 Title : SW846 8260
 Last Update : Tue Jun 26 08:45:17 2018

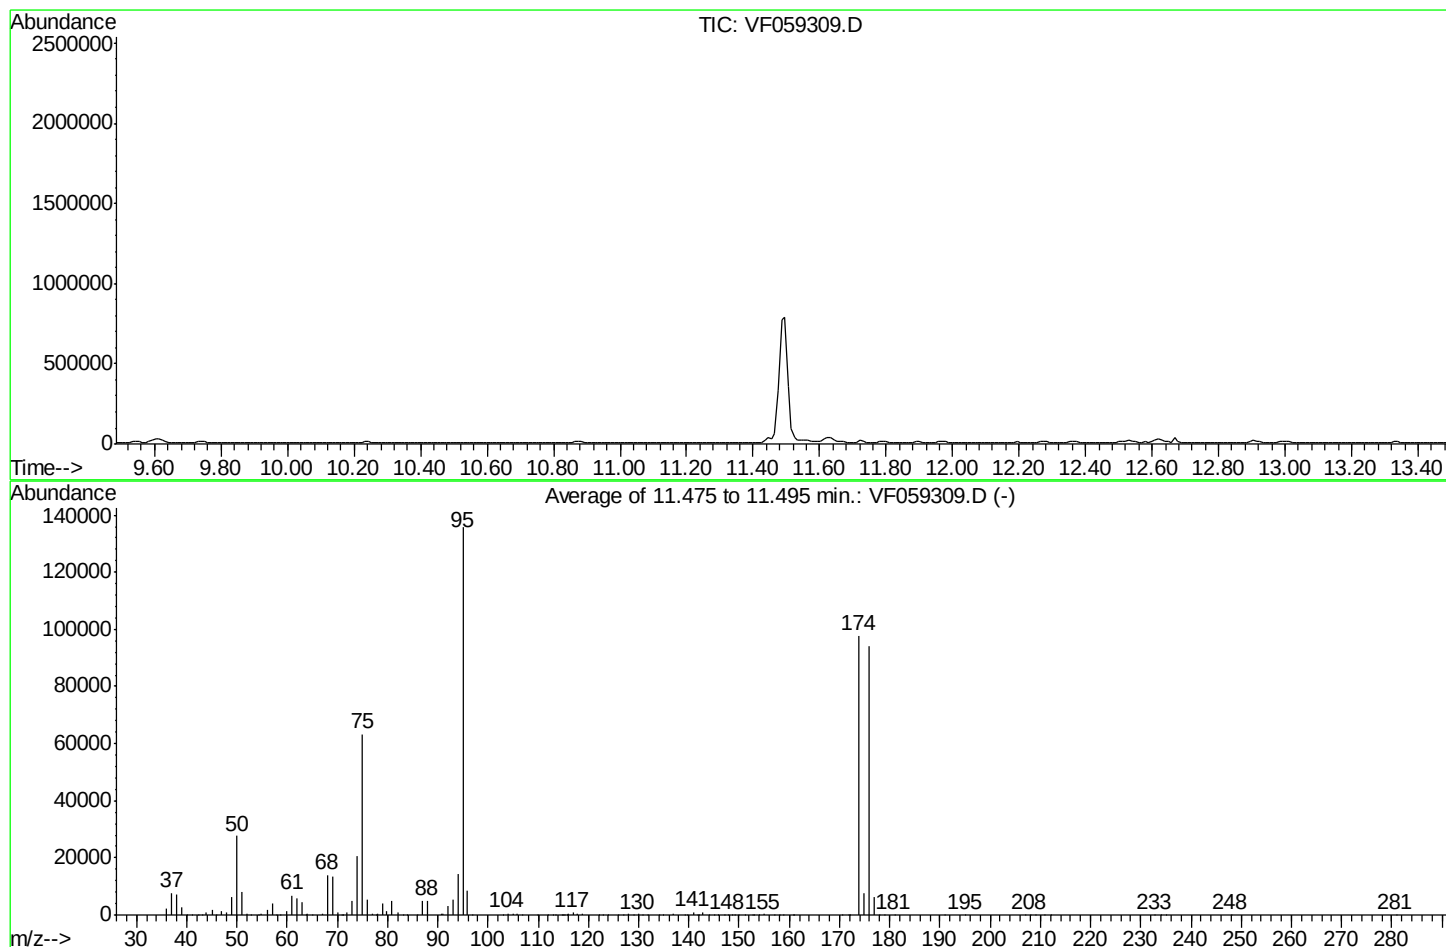

AutoFind: Scans 1110, 1111, 1112; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	27629	PASS
75	95	30	60	46.7	63392	PASS
95	95	100	100	100.0	135714	PASS
96	95	5	9	6.4	8729	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.1	97784	PASS
175	174	5	9	7.6	7475	PASS
176	174	95	101	96.4	94296	PASS
177	176	5	9	6.7	6358	PASS