


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF062718\
 Data File : VF059330.D
 Acq On : 27 Jun 2018 9:47
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F062518S.M
 Title : SW846 8260
 Last Update : Tue Jun 26 08:45:17 2018

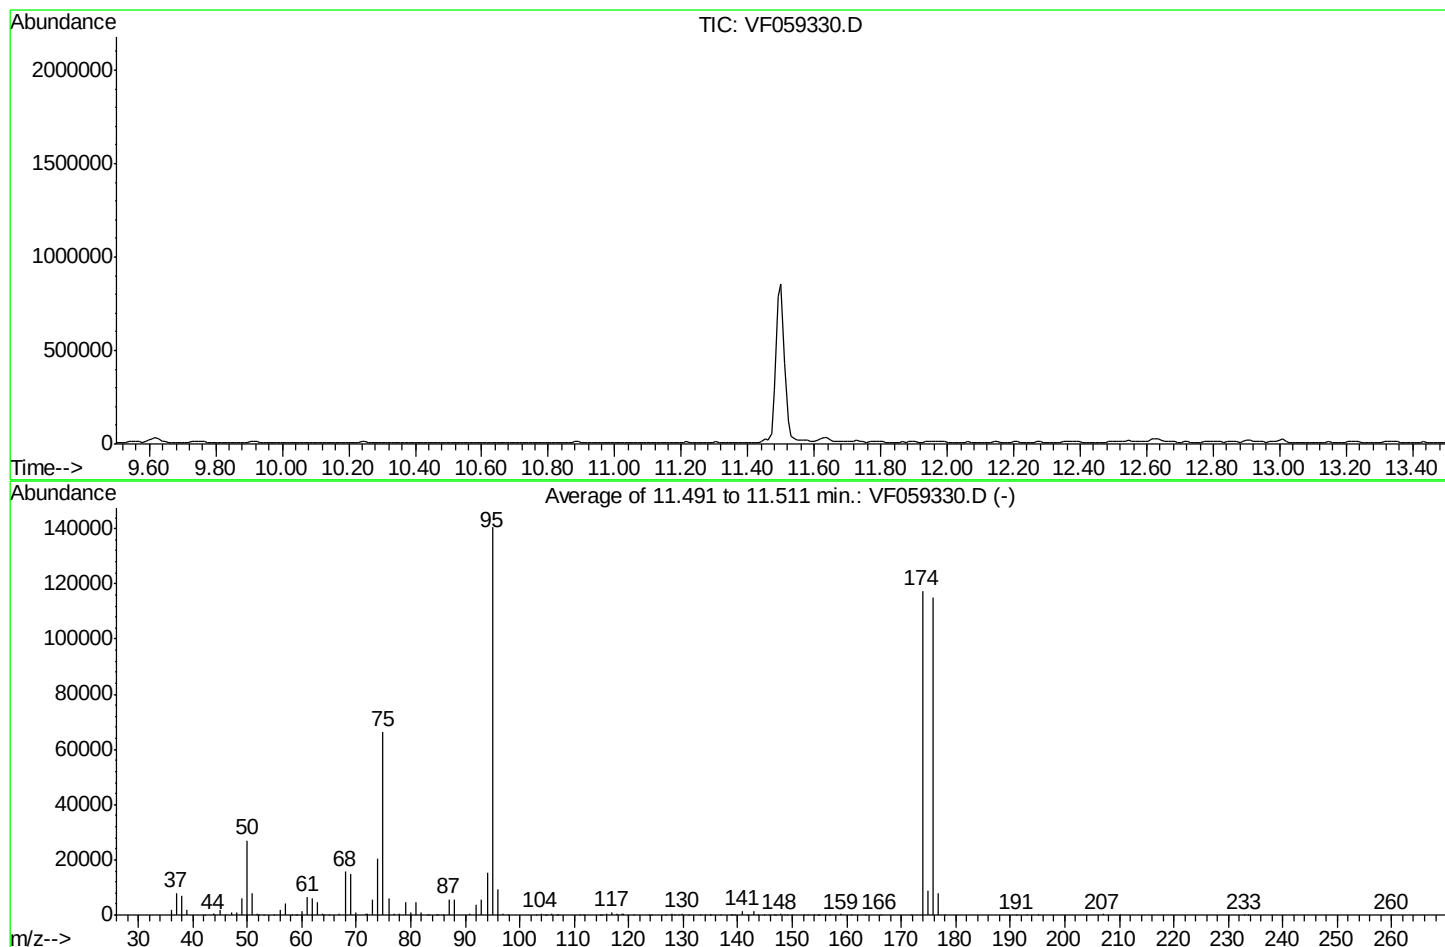

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	27112	PASS
75	95	30	60	47.3	66411	PASS
95	95	100	100	100.0	140464	PASS
96	95	5	9	6.7	9389	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.7	117501	PASS
175	174	5	9	7.6	8916	PASS
176	174	95	101	97.8	114930	PASS
177	176	5	9	6.9	7955	PASS