


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF062818\
 Data File : VF059353.D
 Acq On : 28 Jun 2018 9:48
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F062518S.M
 Title : SW846 8260
 Last Update : Tue Jun 26 08:45:17 2018

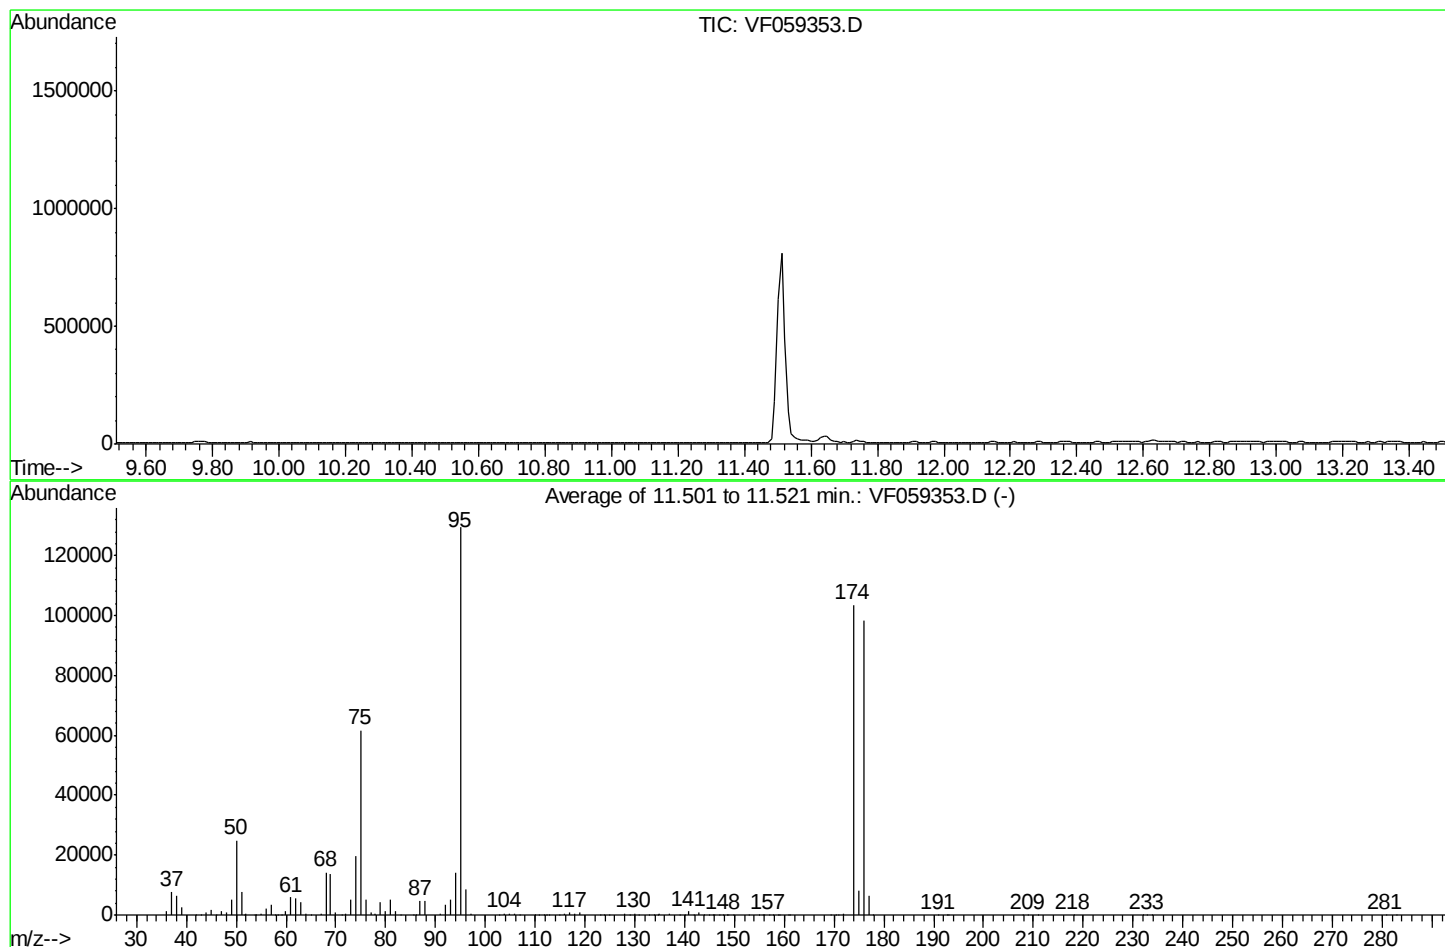

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	24857	PASS
75	95	30	60	47.7	61774	PASS
95	95	100	100	100.0	129434	PASS
96	95	5	9	6.6	8491	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.9	103453	PASS
175	174	5	9	7.7	7995	PASS
176	174	95	101	95.0	98309	PASS
177	176	5	9	6.4	6275	PASS