


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF070218\
Data File : VF059382.D
Acq On : 2 Jul 2018 12:29
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F062518S.M
Title : SW846 8260
Last Update : Tue Jun 26 08:45:17 2018

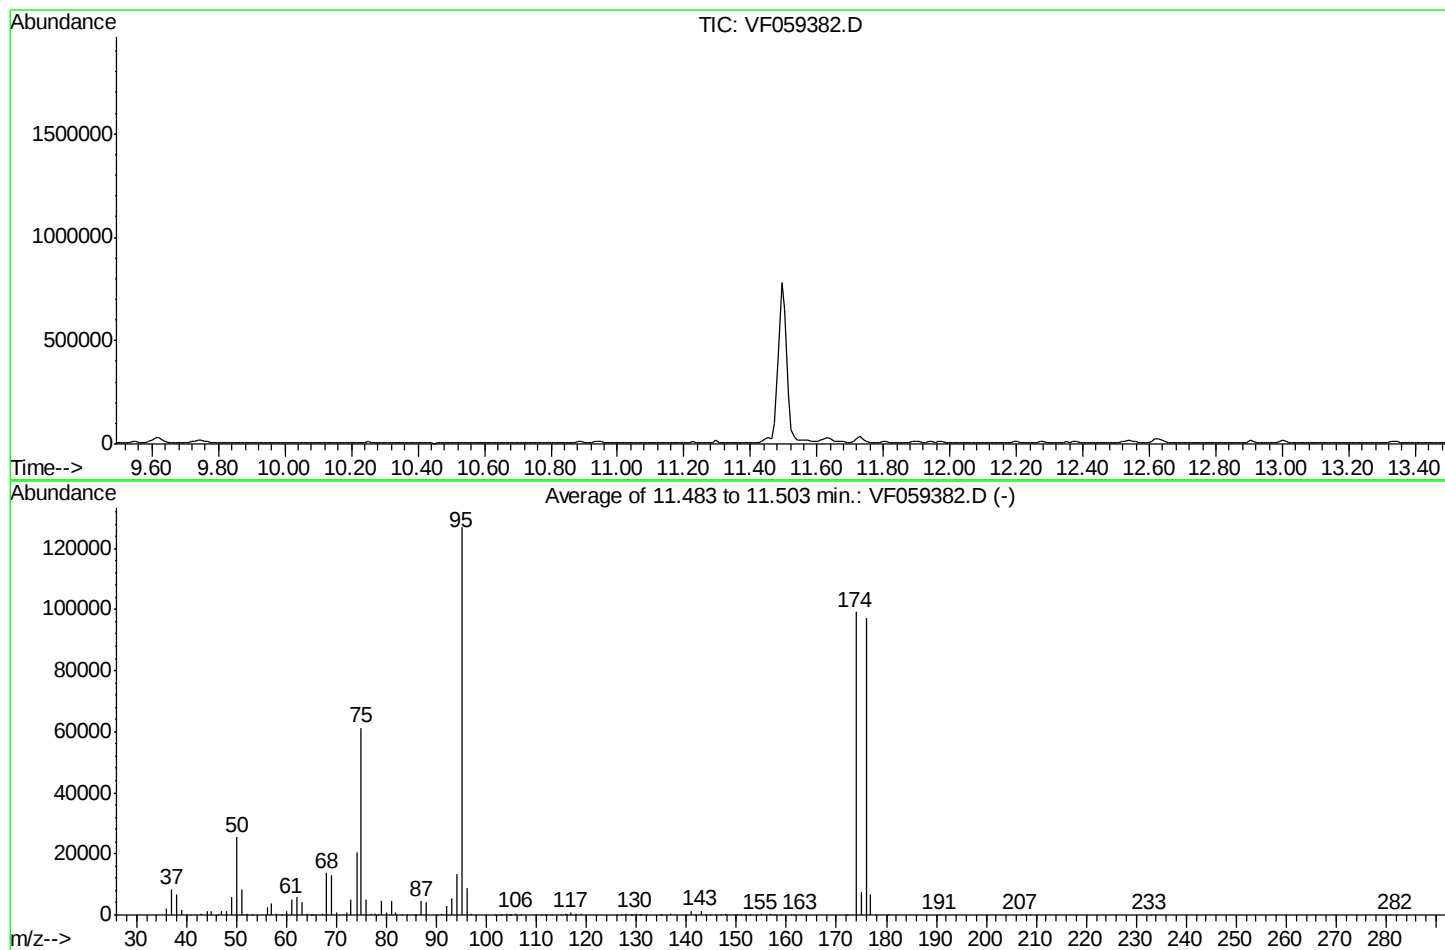

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	25481	PASS
75	95	30	60	48.3	61320	PASS
95	95	100	100	100.0	126904	PASS
96	95	5	9	7.1	8977	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.2	99293	PASS
175	174	5	9	7.5	7433	PASS
176	174	95	101	97.8	97061	PASS
177	176	5	9	6.9	6692	PASS