

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF070618\
 Data File : VF059460.D
 Acq On : 6 Jul 2018 20:07
 Operator : VA/AP
 Sample : J3868-11
 Misc : 5.91g/5mL/MSVOA-F/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 TP-TP-5-S

Quant Time: Jul 07 03:59:33 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F062518S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 26 08:45:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.01	168	194483	50.00	ug/l	-0.02
34) 1,4-Difluorobenzene	5.74	114	291711	50.00	ug/l	-0.02
63) Chlorobenzene-d5	9.90	117	265689	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.62	152	133048	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.99	65	159343	63.42	ug/l	-0.02
Spiked Amount	50.000		Recovery	=	126.84%	
35) Dibromofluoromethane	4.27	113	137813	64.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	129.32%	
50) Toluene-d8	7.68	98	284607	53.93	ug/l	-0.02
Spiked Amount	50.000		Recovery	=	107.86%	
62) 4-Bromofluorobenzene	11.50	95	136417	45.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.66%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF070618\
Data File : VF059460.D
Acq On : 6 Jul 2018 20:07
Operator : VA/AP
Sample : J3868-11
Misc : 5.91g/5mL/MSVOA-F/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
TP-TP-5-S

Quant Time: Jul 07 03:59:33 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F062518S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 26 08:45:17 2018
Response via : Initial Calibration

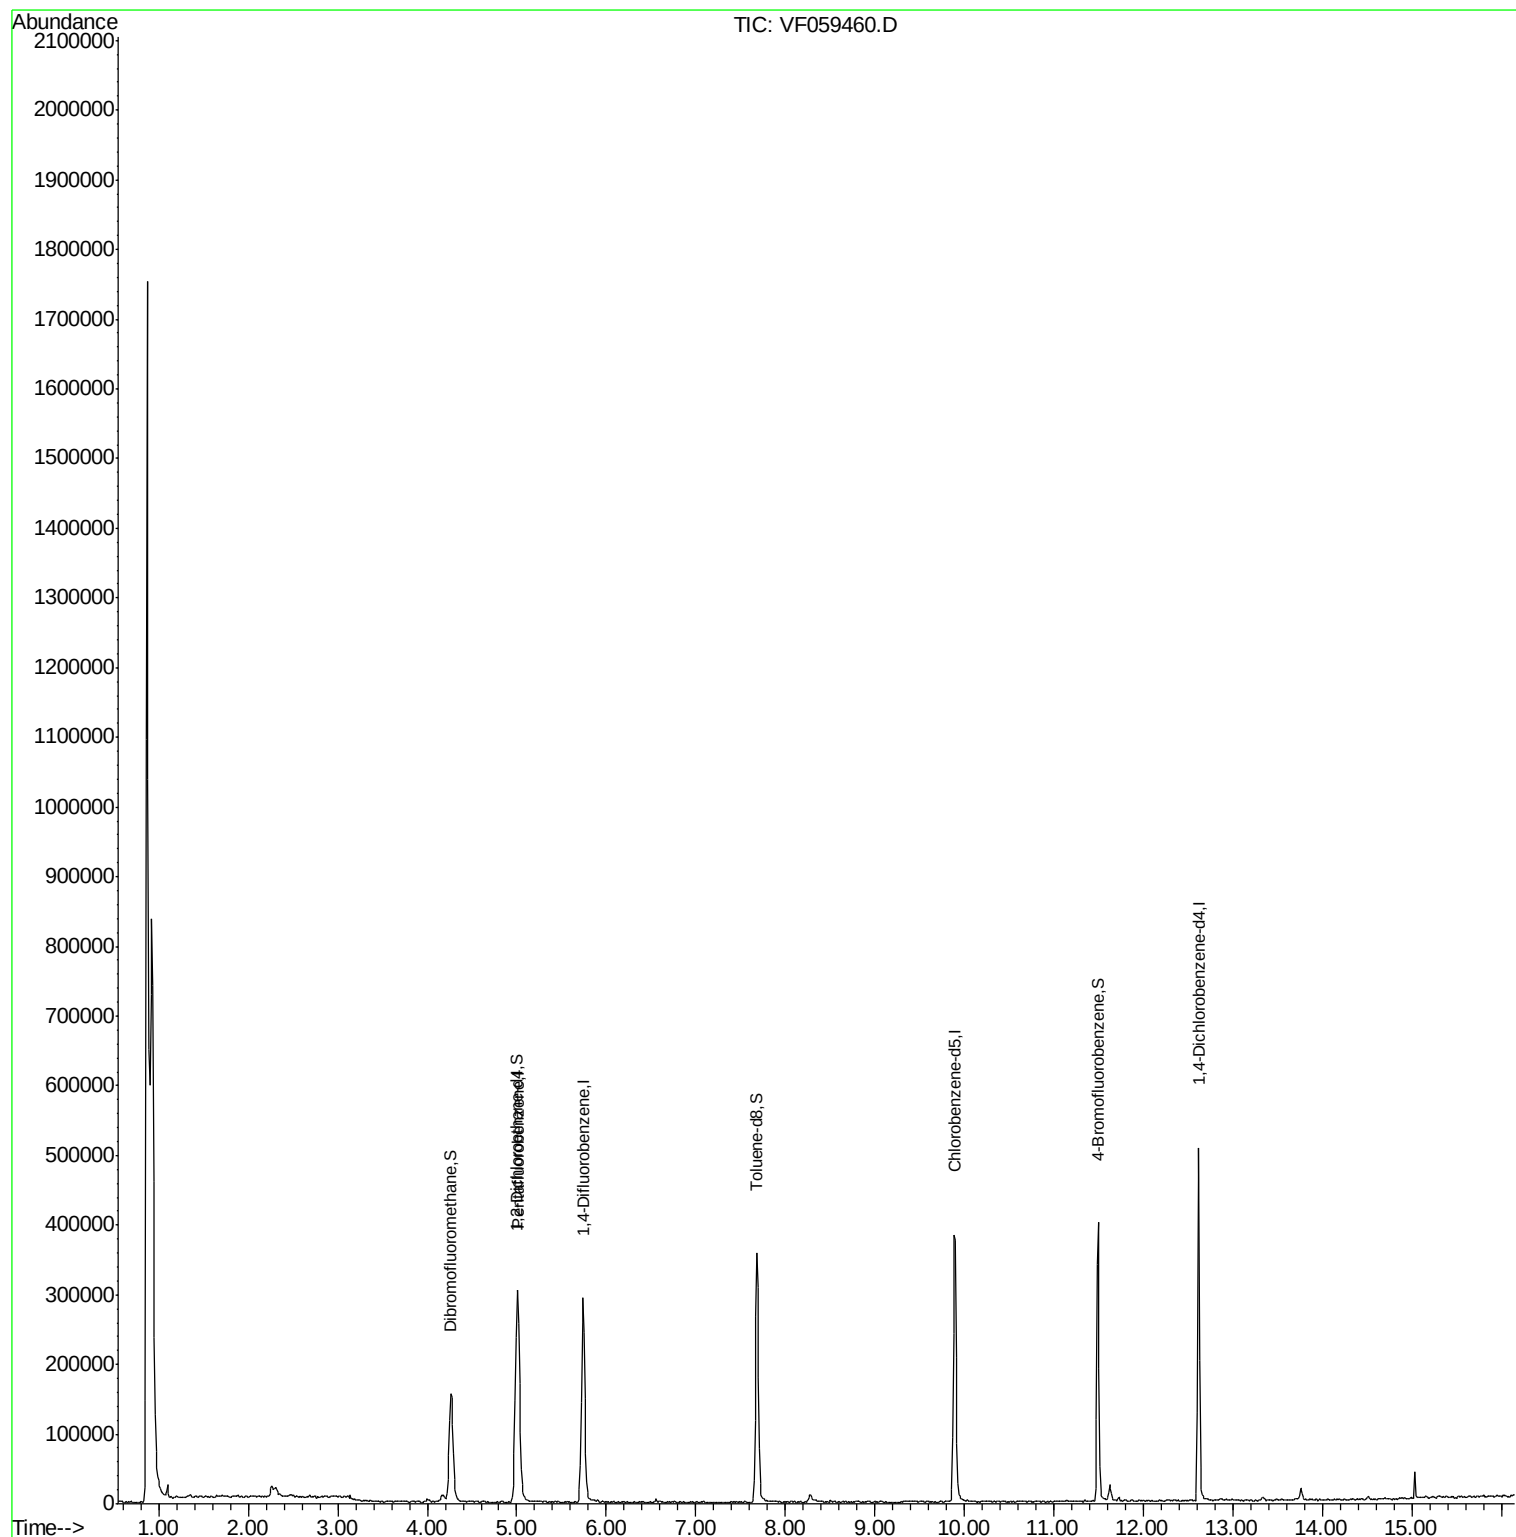

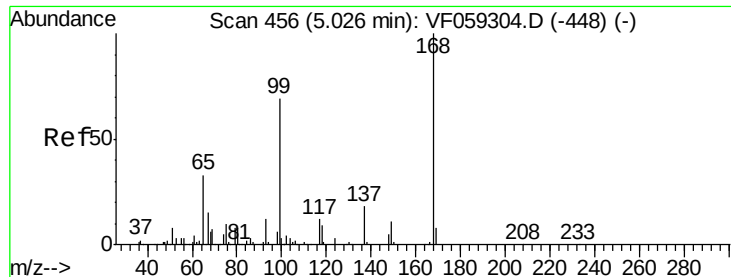

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.01 min Scan# 454

Delta R.T. -0.02 min

Lab File: VF059460.D

Acq: 6 Jul 2018 20:07

Instrument :

MSVOA_F

ClientSampleId :


TP-TP-5-S

Tot Ion:168 Resp: 194483

Ion Ratio Lower Upper




168 100

99 73.0 54.9 82.3

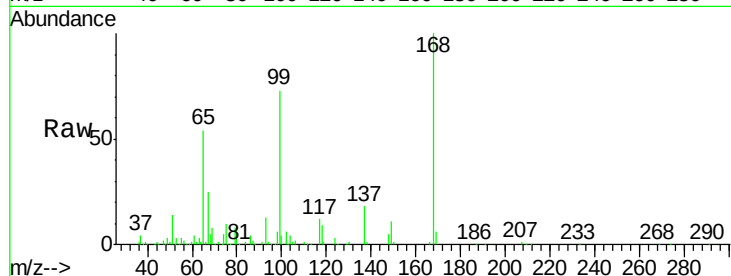

Abundance Ion 168.00 (167.70 to 168.70): V

Ion 99.00 (98.70 to 99.70): VF0

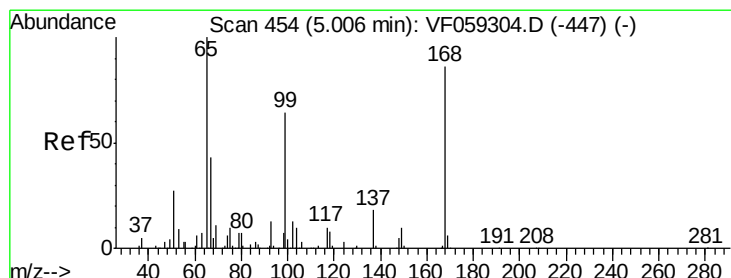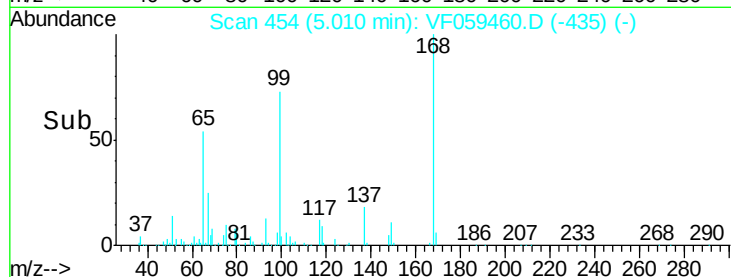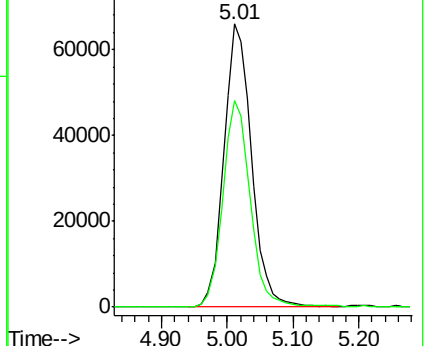

#33

1,2-Dichloroethane-d4

Concen: 63.42 ug/l

RT: 4.99 min Scan# 452

Delta R.T. -0.02 min

Lab File: VF059460.D


Acq: 6 Jul 2018 20:07

Tgt Ion: 65 Resp: 159343

Ion Ratio Lower Upper



65 100


67 42.2 0.0 96.8

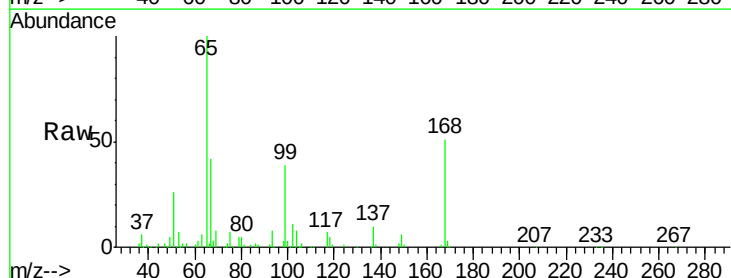

Abundance Ion 65.00 (64.70 to 65.70): VF0

Ion 67.00 (66.70 to 67.70): VF0

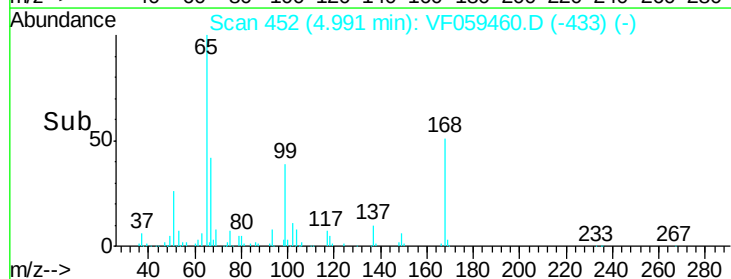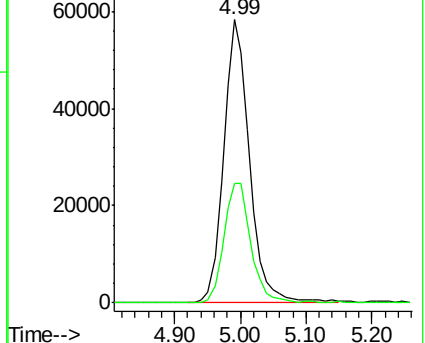

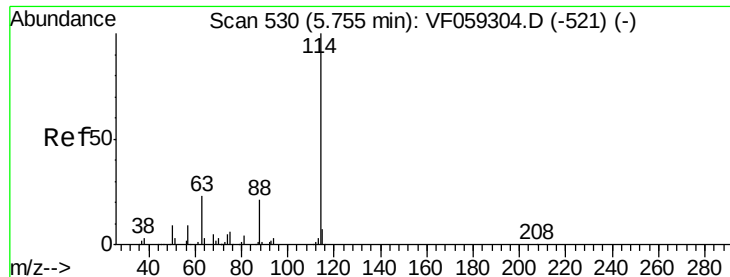

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 5.74 min Scan# 528

Delta R.T. -0.02 min

Lab File: VF059460.D

Acq: 6 Jul 2018 20:07

Instrument :

MSVOA_F

ClientSampleId :

TP-TP-5-S


Tot Ion:114 Resp: 291711

Ion Ratio Lower Upper

114 100

63 23.3 0.0 45.8




88 22.7 0.0 41.2

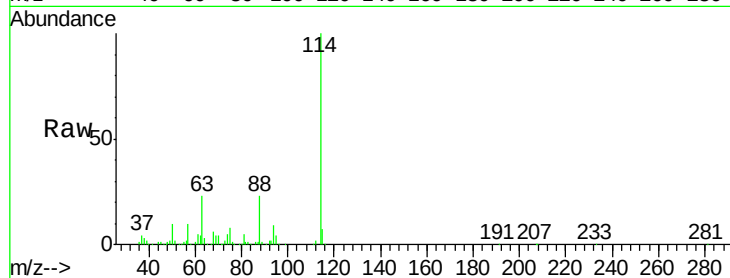

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 88.00 (87.70 to 88.70): VF0

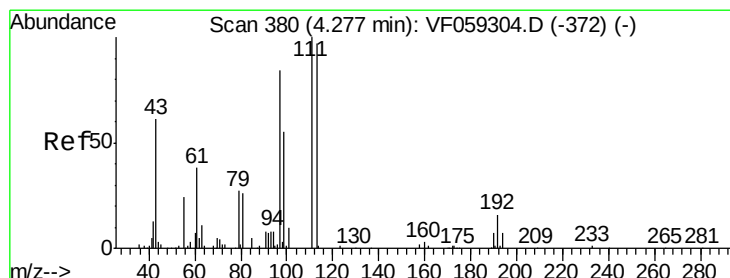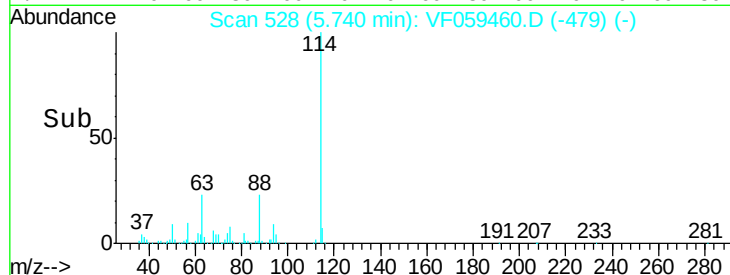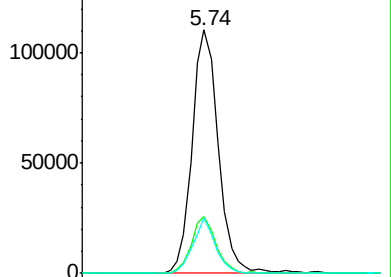

#35

Dibromofluoromethane

Concen: 64.66 ug/l

RT: 4.27 min Scan# 379

Delta R.T. -0.01 min

Lab File: VF059460.D

Acq: 6 Jul 2018 20:07


Tgt Ion:113 Resp: 137813

Ion Ratio Lower Upper

113 100

111 92.9 82.1 123.1



192 16.6 13.0 19.6

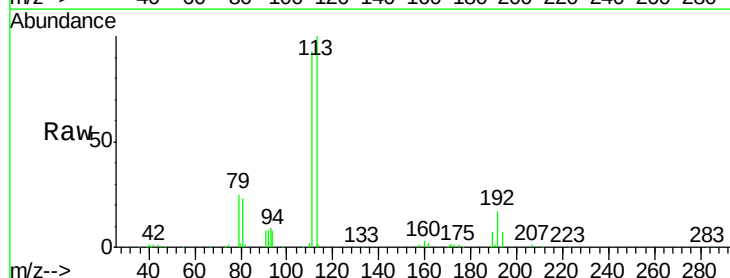


Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V



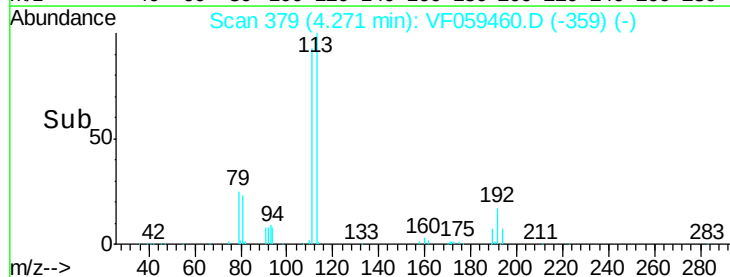
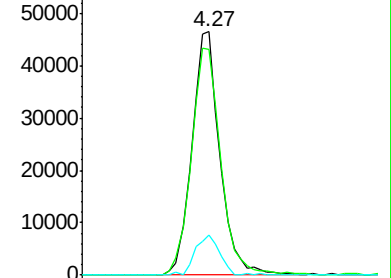


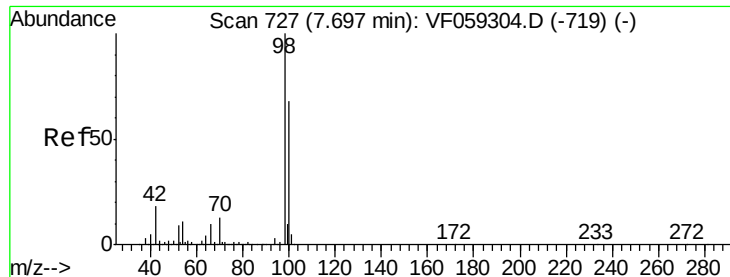

#50
Toluene-d8
Concen: 53.93 ug/l
RT: 7.68 min Scan# 725
Delta R.T. -0.02 min
Lab File: VF059460.D
Acq: 6 Jul 2018 20:07




Instrument :
MSVOA_F
ClientSampleId :
TP-TP-5-S


Tot Ion: 98 Resp: 284607
Ion Ratio Lower Upper
98 100
100 66.3 54.6 82.0

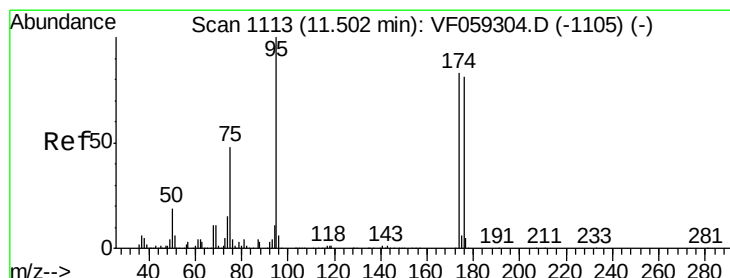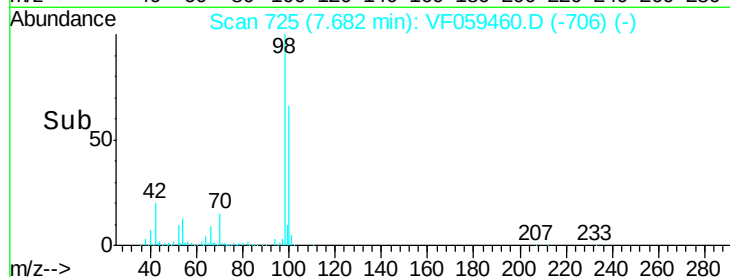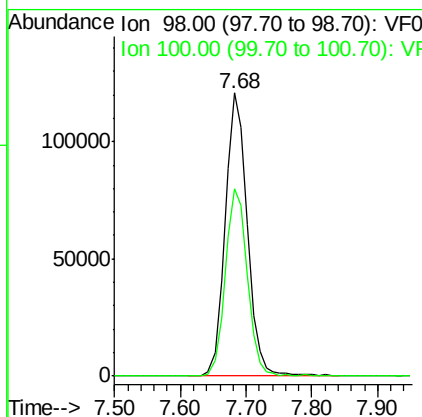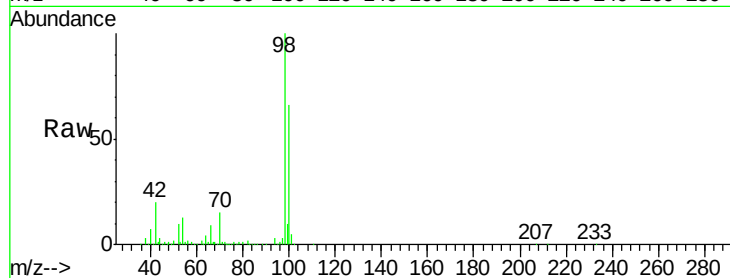

#62
4-Bromofluorobenzene
Concen: 45.83 ug/l
RT: 11.50 min Scan# 1112
Delta R.T. -0.01 min
Lab File: VF059460.D
Acq: 6 Jul 2018 20:07

Tgt Ion: 95 Resp: 136417
Ion Ratio Lower Upper
95 100
174 88.5 0.0 165.2
176 85.2 0.0 161.0

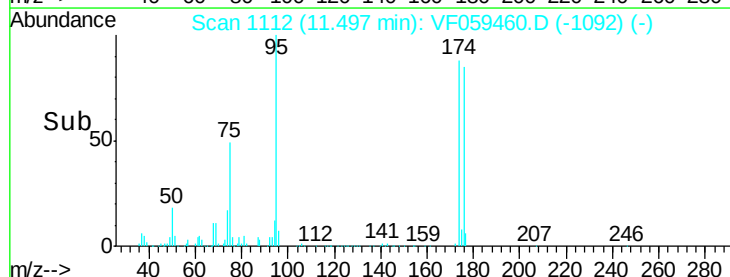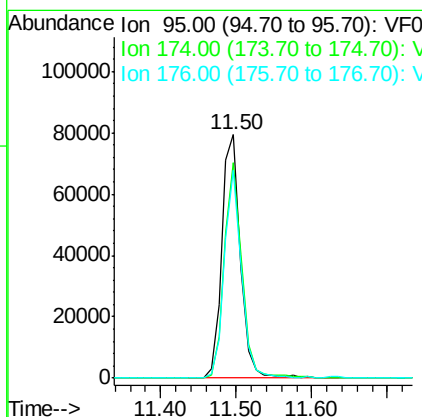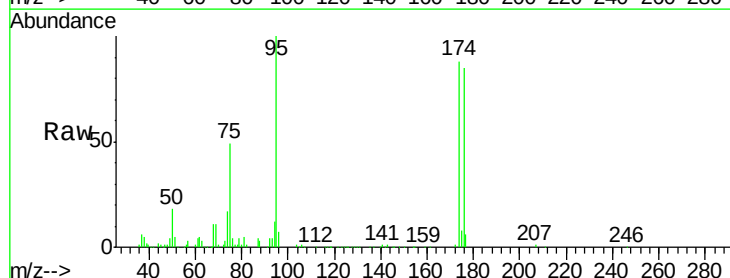


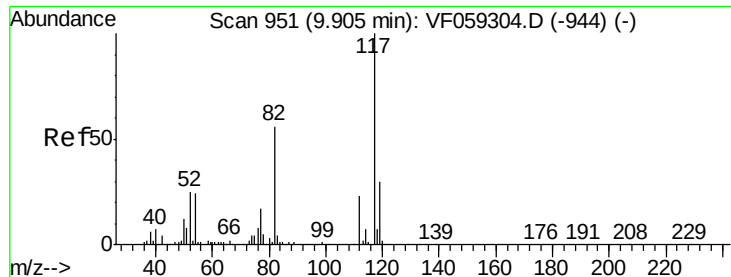




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.90 min Scan# 950
Delta R.T. -0.01 min
Lab File: VF059460.D
Acq: 6 Jul 2018 20:07

Instrument :
MSVOA_F
ClientSampleId :
TP-TP-5-S

Tot Ion	Ratio	Lower	Upper
117	100		
82	58.9	44.6	66.8
119	32.9	24.1	36.1

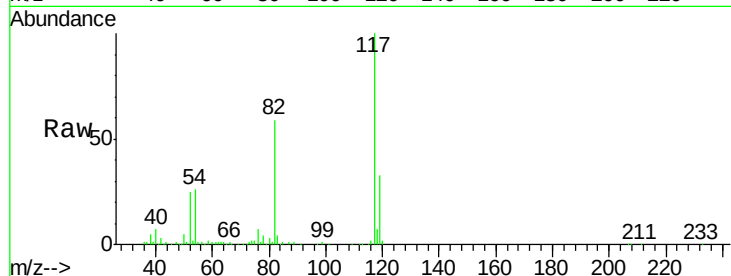


Abundance Ion 117.00 (116.70 to 117.70): V
Ion 82.00 (81.70 to 82.70): V
Ion 119.00 (118.70 to 119.70): V

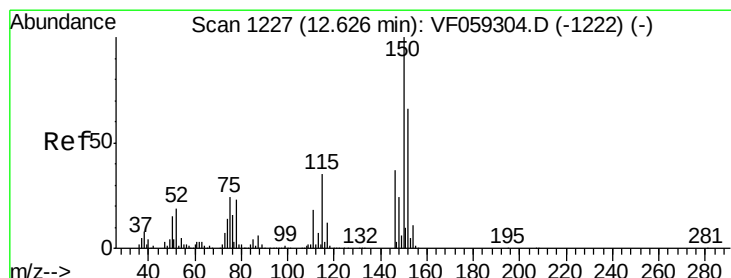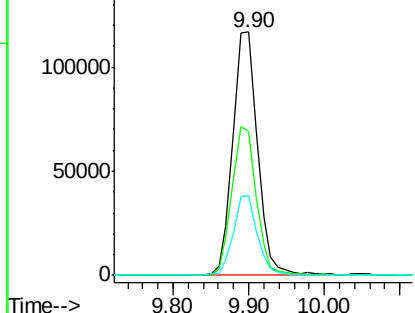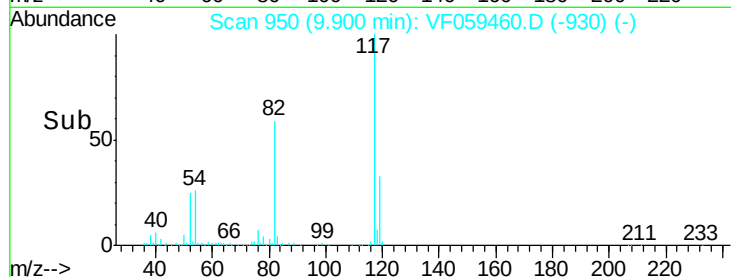

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.62 min Scan# 1226
Delta R.T. -0.01 min
Lab File: VF059460.D
Acq: 6 Jul 2018 20:07

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.1	27.1	81.3
150	153.3	0.0	305.2

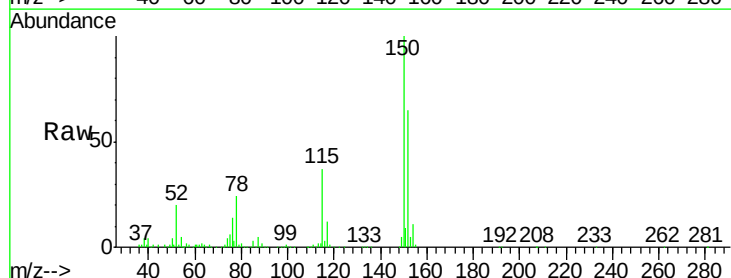

Abundance Ion 152.00 (151.70 to 152.70): V
Ion 115.00 (114.70 to 115.70): V
Ion 150.00 (149.70 to 150.70): V

