


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF070718\
 Data File : VF059469.D
 Acq On : 7 Jul 2018 00:42
 Operator : VA/AP
 Sample : BFB
 Misc : 5.03g/5mL/MSVOA-F/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F070718S.M
 Title : SW846 8260
 Last Update : Sat Jul 07 06:35:36 2018

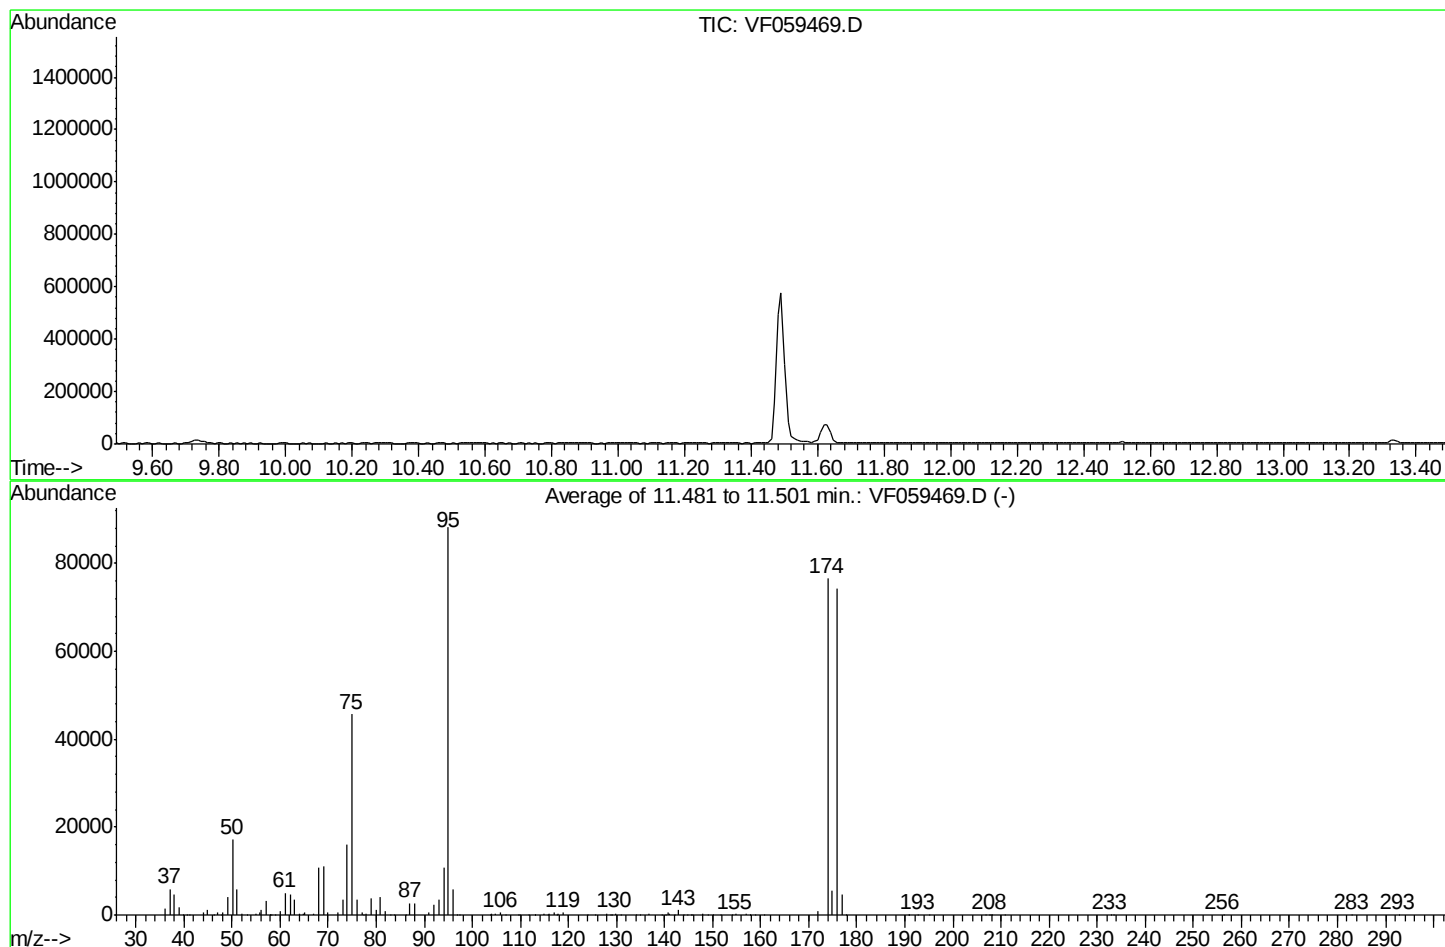

AutoFind: Scans 1111, 1112, 1113; Background Corrected with Scan 1105

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	17127	PASS
75	95	30	60	51.8	45722	PASS
95	95	100	100	100.0	88242	PASS
96	95	5	9	6.5	5701	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.7	76517	PASS
175	174	5	9	7.1	5415	PASS
176	174	95	101	97.1	74314	PASS
177	176	5	9	6.4	4739	PASS