


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF071818\
 Data File : VF059518.D
 Acq On : 18 Jul 2018 17:03
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F071718S.M
 Title : SW846 8260
 Last Update : Wed Jul 18 04:09:10 2018

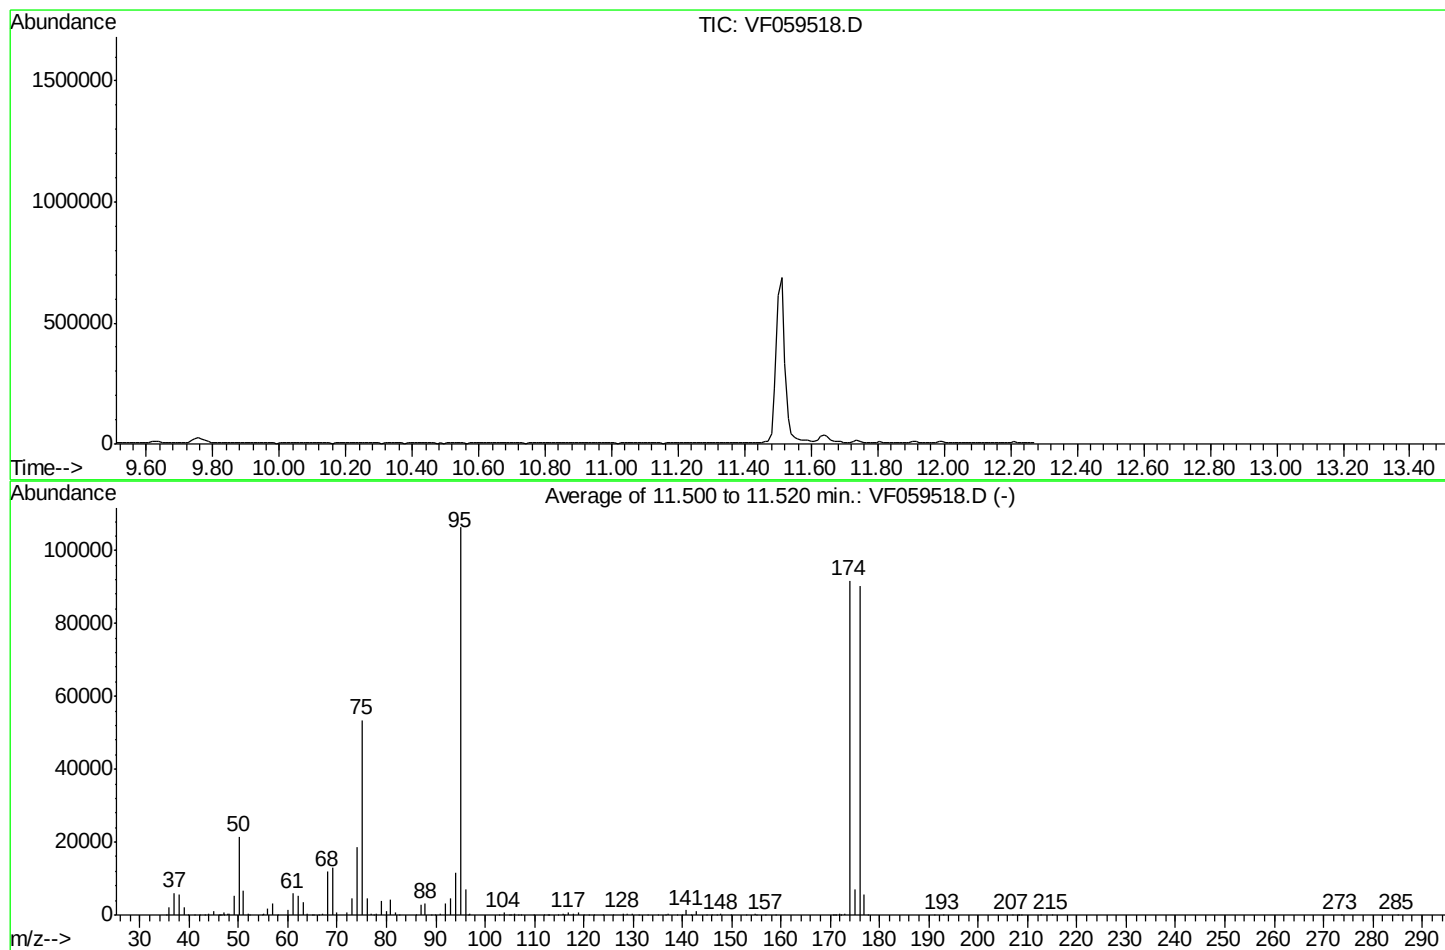

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	21598	PASS
75	95	30	60	50.4	53568	PASS
95	95	100	100	100.0	106373	PASS
96	95	5	9	6.6	7005	PASS
173	174	0.00	2	0.2	226	PASS
174	95	50	100	86.3	91826	PASS
175	174	5	9	7.7	7050	PASS
176	174	95	101	98.1	90114	PASS
177	176	5	9	6.3	5722	PASS