


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF071918\
 Data File : VF059542.D
 Acq On : 19 Jul 2018 5:29
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F071718S.M
 Title : SW846 8260
 Last Update : Wed Jul 18 04:09:10 2018

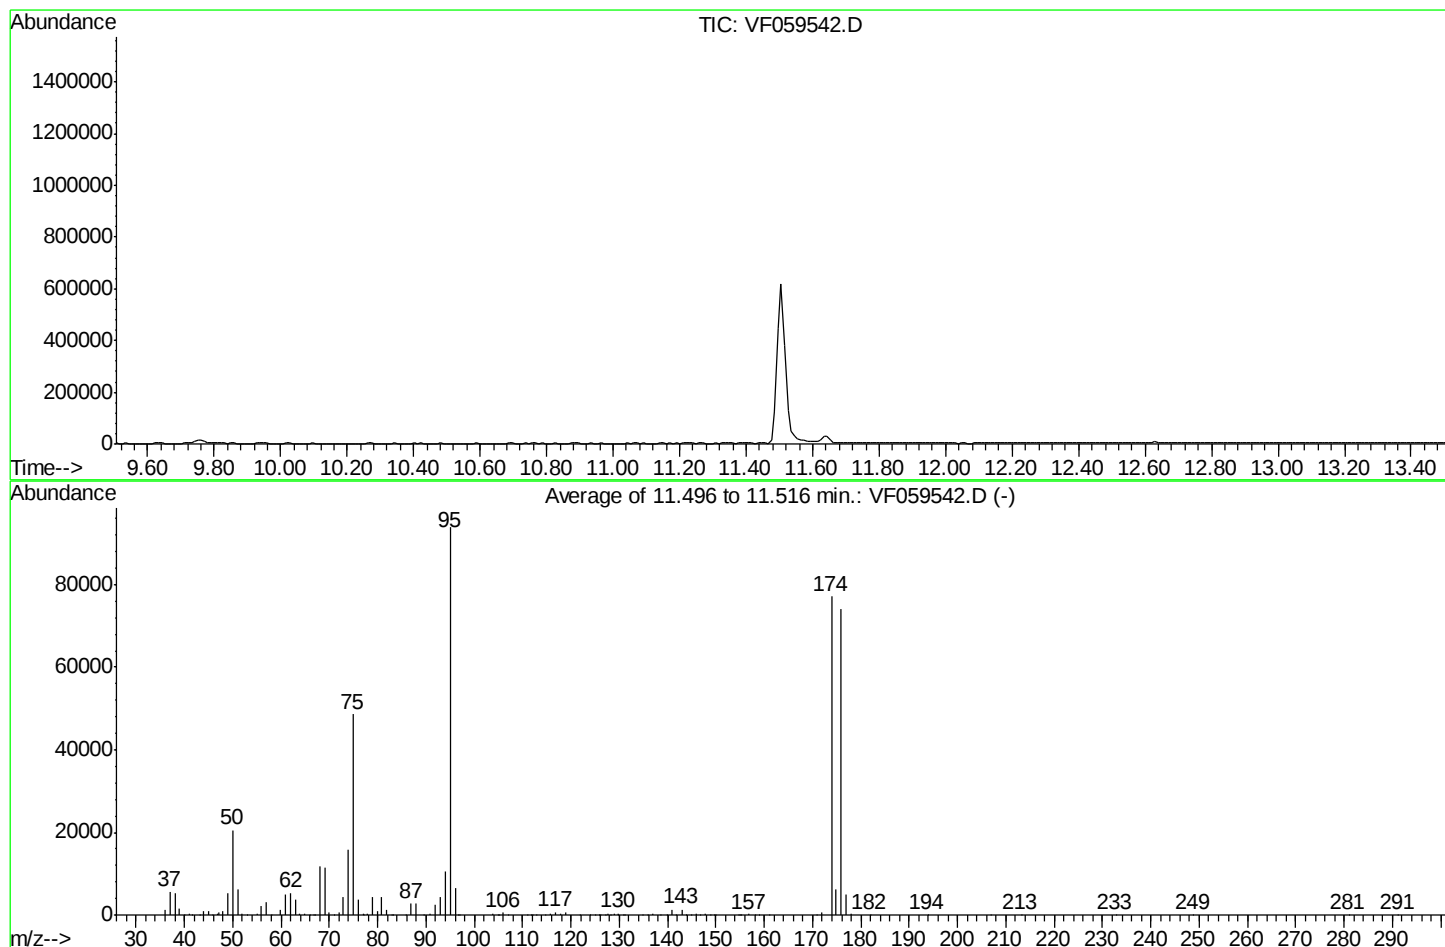

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	20466	PASS
75	95	30	60	51.8	48592	PASS
95	95	100	100	100.0	93896	PASS
96	95	5	9	6.9	6445	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.2	77144	PASS
175	174	5	9	7.9	6126	PASS
176	174	95	101	96.1	74136	PASS
177	176	5	9	6.7	4962	PASS