


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF072018\
Data File : VF059587.D
Acq On : 20 Jul 2018 16:40
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F071718S.M
Title : SW846 8260
Last Update : Wed Jul 18 04:09:10 2018

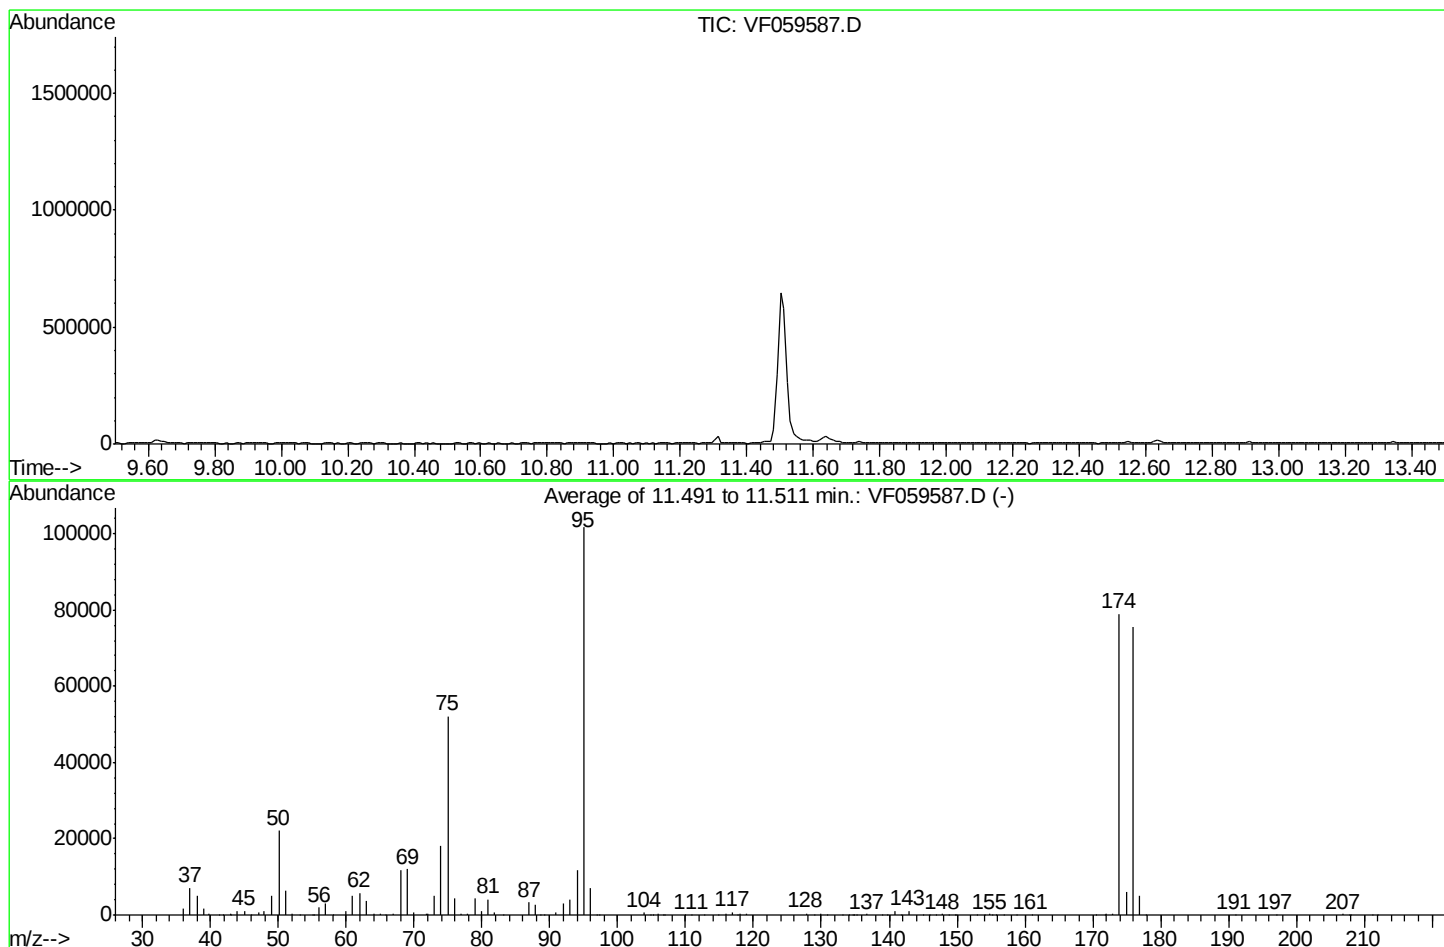

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	22011	PASS
75	95	30	60	51.3	52152	PASS
95	95	100	100	100.0	101669	PASS
96	95	5	9	6.8	6922	PASS
173	174	0.00	2	0.3	233	PASS
174	95	50	100	77.7	79024	PASS
175	174	5	9	7.7	6083	PASS
176	174	95	101	95.5	75485	PASS
177	176	5	9	6.9	5176	PASS