


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF072318\
Data File : VF059609.D
Acq On : 23 Jul 2018 12:19
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F072318S.M
Title : SW846 8260
Last Update : Tue Jul 24 04:17:55 2018

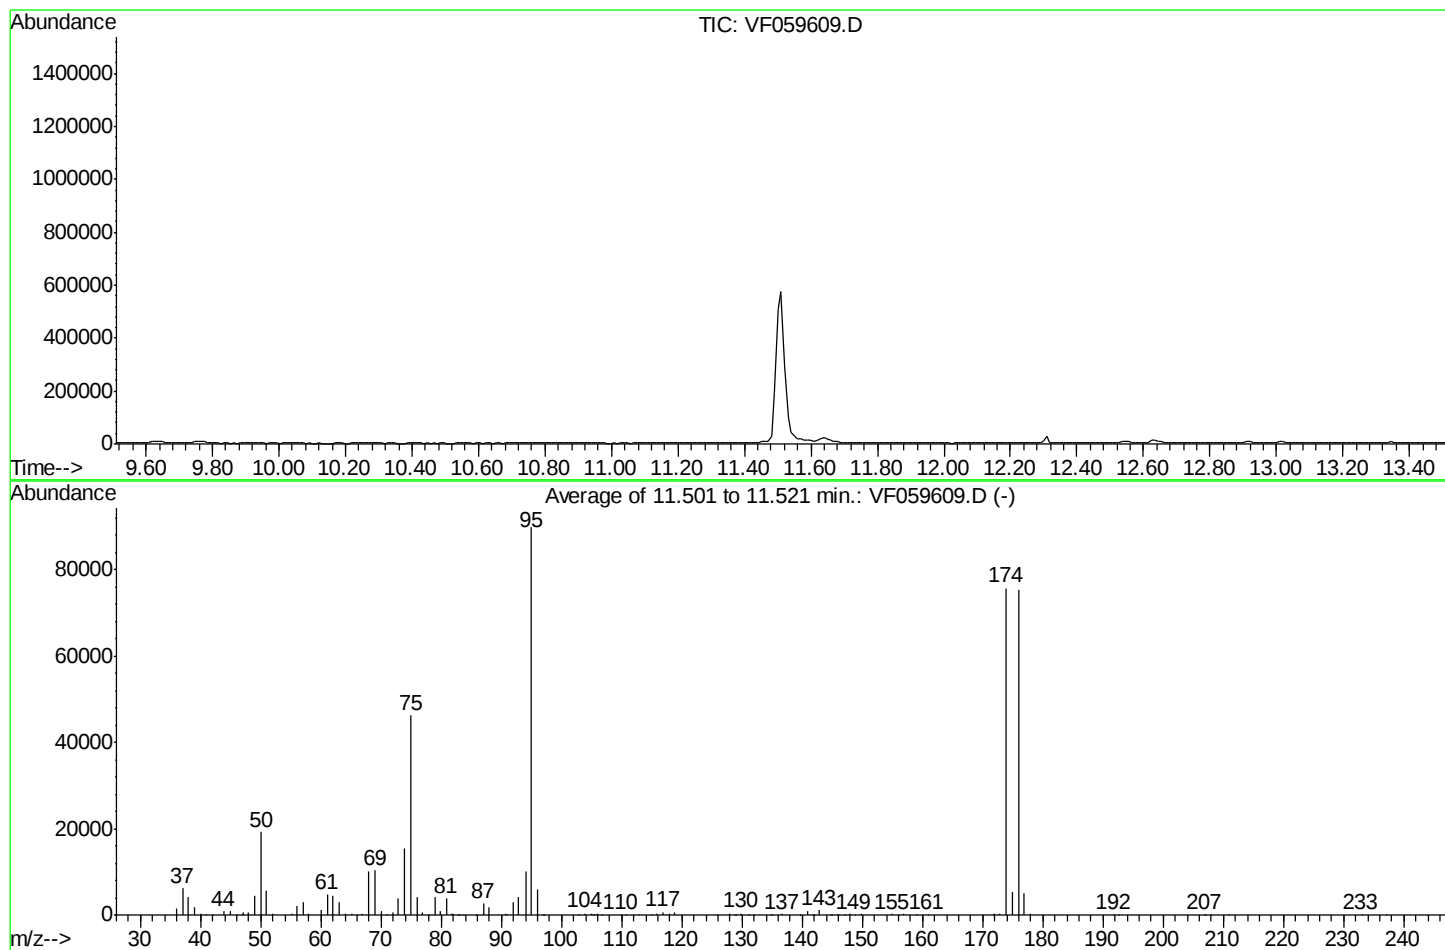

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	19165	PASS
75	95	30	60	51.4	46146	PASS
95	95	100	100	100.0	89746	PASS
96	95	5	9	6.6	5916	PASS
173	174	0.00	2	0.3	238	PASS
174	95	50	100	84.3	75637	PASS
175	174	5	9	7.1	5407	PASS
176	174	95	101	99.7	75381	PASS
177	176	5	9	6.8	5108	PASS