


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF072418\
Data File : VF059633.D
Acq On : 24 Jul 2018 15:03
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F072418S.M
Title : SW846 8260
Last Update : Wed Jul 25 02:29:31 2018

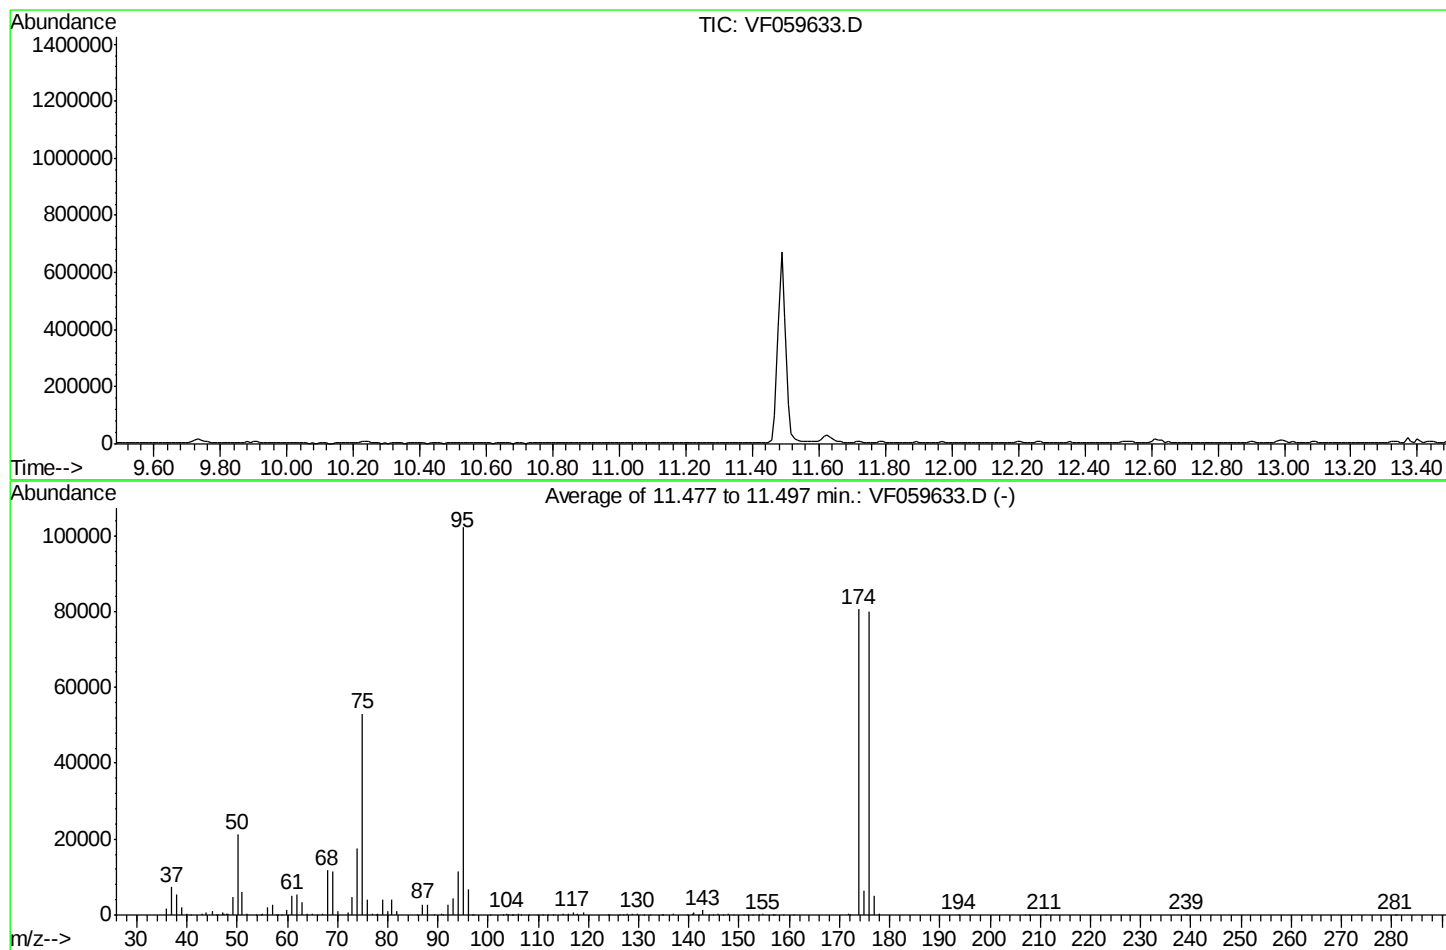

AutoFind: Scans 1110, 1111, 1112; Background Corrected with Scan 1104

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	21113	PASS
75	95	30	60	51.9	53090	PASS
95	95	100	100	100.0	102200	PASS
96	95	5	9	6.6	6749	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.8	80544	PASS
175	174	5	9	7.8	6317	PASS
176	174	95	101	99.3	79978	PASS
177	176	5	9	6.5	5202	PASS