


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF073118\
Data File : VF059699.D
Acq On : 31 Jul 2018 9:50
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F073018S.M
Title : SW846 8260
Last Update : Tue Jul 31 15:23:22 2018

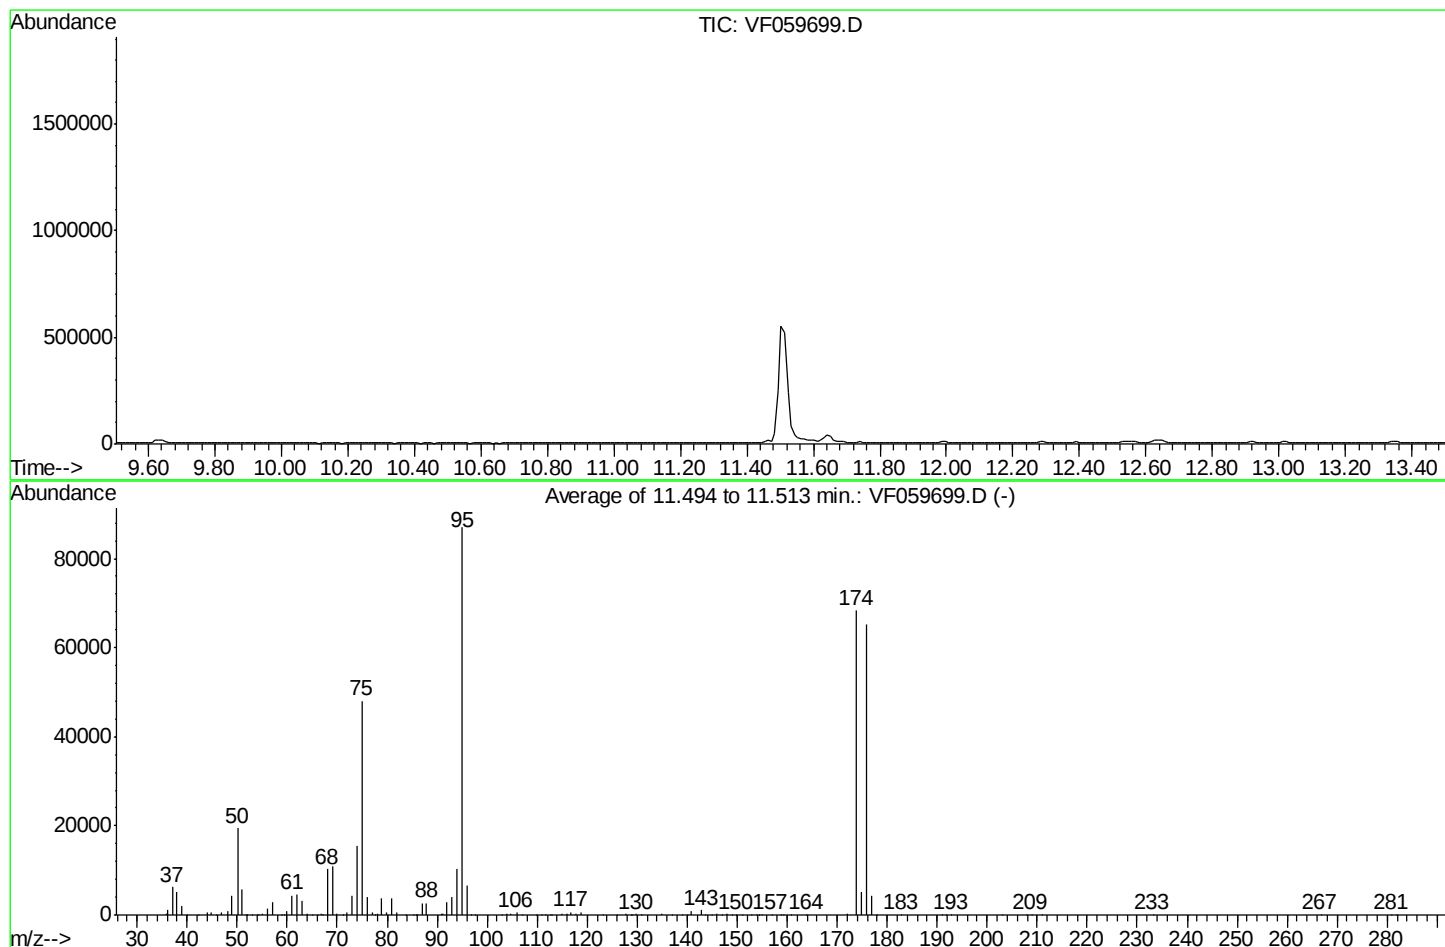

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	19454	PASS
75	95	30	60	55.2	47997	PASS
95	95	100	100	100.0	87005	PASS
96	95	5	9	7.6	6583	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.4	68248	PASS
175	174	5	9	7.7	5231	PASS
176	174	95	101	95.6	65224	PASS
177	176	5	9	6.7	4350	PASS