


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF080118\
 Data File : VF059773.D
 Acq On : 2 Aug 2018 00:18
 Operator : VA/AP
 Sample : BFB
 Misc : 5a/5mL/MSVOA F/SOIL
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F073018S.M
 Title : SW846 8260
 Last Update : Tue Jul 31 15:23:22 2018

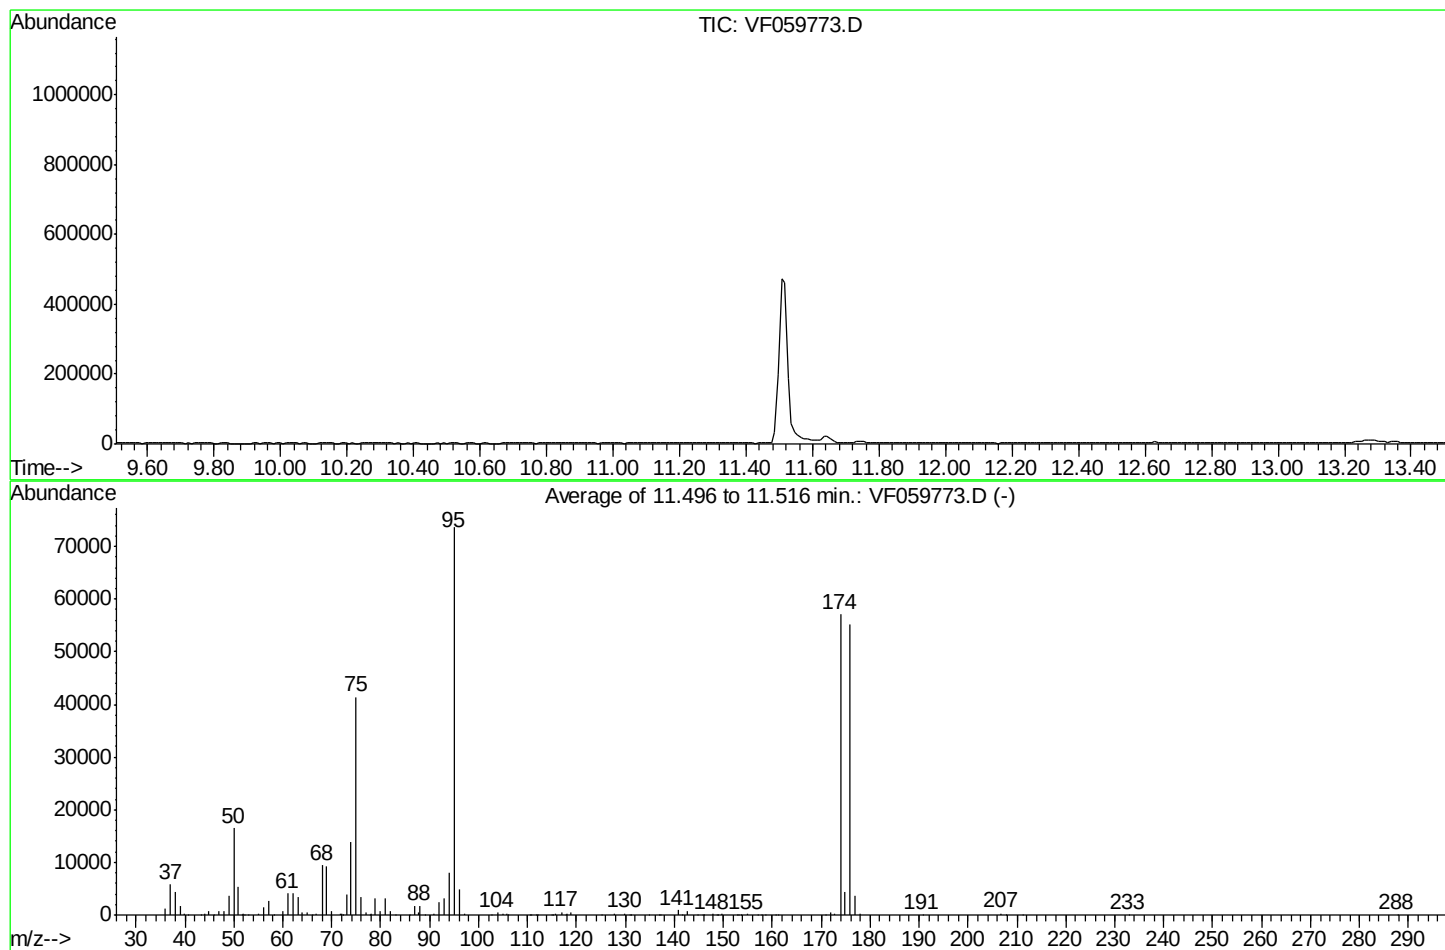

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	16467	PASS
75	95	30	60	56.3	41456	PASS
95	95	100	100	100.0	73634	PASS
96	95	5	9	6.5	4763	PASS
173	174	0.00	2	0.6	346	PASS
174	95	50	100	77.6	57122	PASS
175	174	5	9	7.5	4290	PASS
176	174	95	101	96.7	55253	PASS
177	176	5	9	6.6	3641	PASS